





[CAD-CAM solutions]

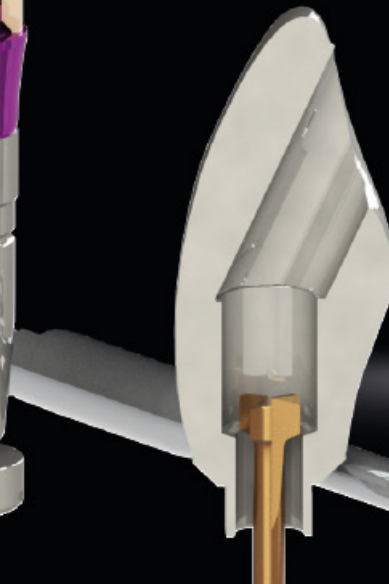

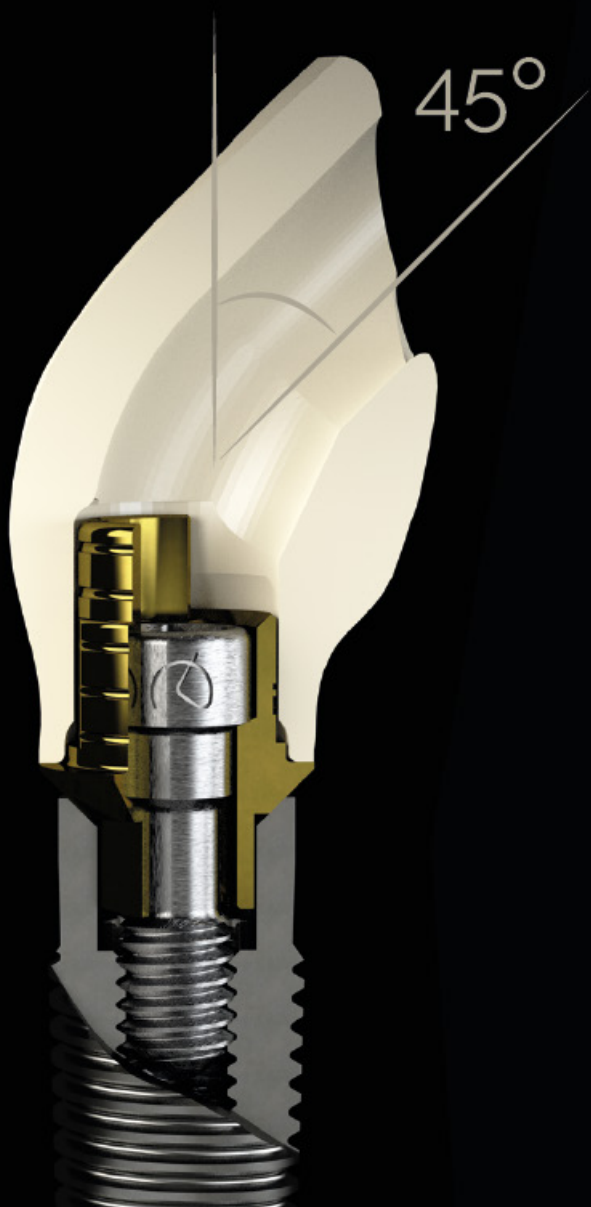

www.dynamicabutment.com

DYNAMIC ABUTMENT® SOLUTIONS

VIRGINIA WOOLF, 17 · 25005 · LLEIDA (SPAIN)
INTERNATIONAL +34 973 289 580
das@dynamicabutment.com

SPAIN +34 973 289 580
spain@dynamicabutment.com

Dynamic Abutment® Solutions is the trademark of the manufacturer Talladium España S.L

The information included in this catalogue is exclusively addressed to professionals in dental sector.

All commercial trademarks mentioned herein are fully registered by their respective companies, and the images that appear are just to provide an orientation.

Talladium reserves the right to modify this document without previous notice.

Talladium is not responsible for the inadequate execution of these products if the warning indications corresponding to every reference are not contemplated.

All of the products listed in this brochure are marking in accordance with CE legislation. Some of the products are not authorized for sale and distribution or do not have a sales license in some countries according to other legislations (FDA, CMDCAS, etc.) Please ask for information: das@dynamicabutment.com

 Marking in accordance with CE legislation and applicable sanitary regulations



Visit our Online Store to find all our products and compatibilities :

www.dynamicabutmentstore.com

4	DYNAMIC ABUTMENT® SOLUTIONS
5	RESEARCH & DEVELOPMENT
6	QUALITY CENTER
7	INTERNATIONAL CUSTOMER SERVICE
8	DYNAMIC SYSTEM
10	DYNAMIC SYSTEM FOR MILLING STRUCTURES
12	CADCAM WORKFLOW - DAS PRODUCTS
14	DYNAMIC μSCANBODY/ ADAPTOR
16	LAB SCANBODY
17	SCANALOG
18	DYNAMIC TIBASE®/DYNAMIC 3TIBASE®
20	DYNAMIC TIBASE® GINGIVAL OPTIONS
22	DYNAMIC PREMILL3D®/ADAPTORS
24	DYNAMIC MILLING TOOL - DMTONE®
26	DIGITAL ANALOG
28	DAS LIBRARIES
30	DAS CUSTOMIZED SERVICES
32	CAD-CAM
36	DYNAMIC SYSTEM - LIST OF COMPATIBILITES
52	DYNAMIC SYSTEM COMPATIBILITES
168	DYNAMIC SCREWS TECHNICAL SPECIFICATIONS
171	DYNAMIC SCREWDRIVER & DYNAMIC SCREWS
172	STRAIGHT SCREWS TECHNICAL SPECIFICATIONS
175	SCREWDRIVERS & STRAIGHT SCREWS
176	INTRAORAL SYSTEM COLORS ACCORDING TO COMPATIBILITY
180	DYNAMIC MILLING TOOL SPECIFICATIONS
182	SCREWDRIVER ADAPTOR/COMPLEMENTS
183	IDENTIFICATION PRODUCT/ SECURITY & TRACEABILITY
184	TALLADIUM GUARANTEE

DYNAMIC ABUTMENT® SOLUTIONS YOUR DIGITAL DENTAL PARTNER

The digital transformation of your company is an essential process for the future of your clinic or laboratory. Adapting to the new technologies, required by this new workflow, is not easy and requires a great effort in terms of both investment and know-how, which involves a detailed planning. Dynamic Abutment Solutions offers you its experience in multiple implementations to offer you a wide range of personalized services for the development of such project, as well as the manufacturing of customized products to adapt to your work protocol.

All Dynamic Abutment Solutions' custom-developed products have the necessary technological support for their correct introduction into the medical device market in accordance with current standards.

We assist you in all the stages of the digital flow in order your work reaches the level of excellence you want; from the initial scanning process to the completion of the prosthetic restoration.

Undoubtedly, DAS is your **digital dental partner**.

RESEARCH & DEVELOPMENT

"Focus on excellence and R&D&I has seen us become No.1 in angled solutions"

The R&D&I Department at Dynamic Abutment® Solutions is endorsed by the UNE 166002 certificate for R&D&I systems management.

It is actively involved in international projects, working alongside the main operators in the sector, contributing know-how in both production and machining and the design of digital hardware for CAD and production management (CAM).

Consequent to this work with the leading figures and companies in the sector, we develop new products that are rolled out from our own Production Center. The Production Center features next-gen equipment, enabling us to make prototypes prior to receiving the final thumbs-up for the product from the R&D&I Department.

The R&D&I Center ensures comprehensive control over all the development stages for new projects, allowing them to be transformed into new products featuring the top-notch safety and quality levels that characterise our output and reaching our clients as soon as possible.



QUALITY CENTER

「 "Controlling our quality process ensures the safety of our products" 」

Dynamic Abutment® Solutions has a Quality Center with the very latest metrology and control, prototyping and physical-chemical treatment equipment, and sanitary areas for refitting and packaging health products in an ISO-8 clean room.

Controlling the whole quality process ensures that our products are measured, inspected and checked using the most advanced control methods in the sector. We guarantee the quality of our products from production all the way through to packaging.

Being present in international markets means we have the mandatory health certificates that cover our product:

CE marking, CMD/CAS regulations, or FDA certificates, among others.

Our primary concern from the very beginning has been the quality and safety of our products: UNE-EN ISO 9001:2015, UNE-EN ISO 13485:2016, and UNE 166002:2014.



INTERNACIONAL CUSTOMER CENTER

「 "Our experience and know-how serving our clients and distributors" 」

The main objective of the exclusive Dynamic Abutment® Solutions Customer Service Center is to maintain a constant channel of communication with our distributors and associates.

Our products are available in over 45 countries across five continents, with guaranteed health product management and certificates for international markets.




We offer our clients technical support, along with immediate answers and solutions with direct support from the R&D&I technical department for even the most complex of cases.

We participate in fairs, events, conferences and training sessions through our distributors and associates.



Direct contact with and suggestions from our clients allows us to continue improving the quality of the products and services we offer.

DYNAMIC SYSTEM

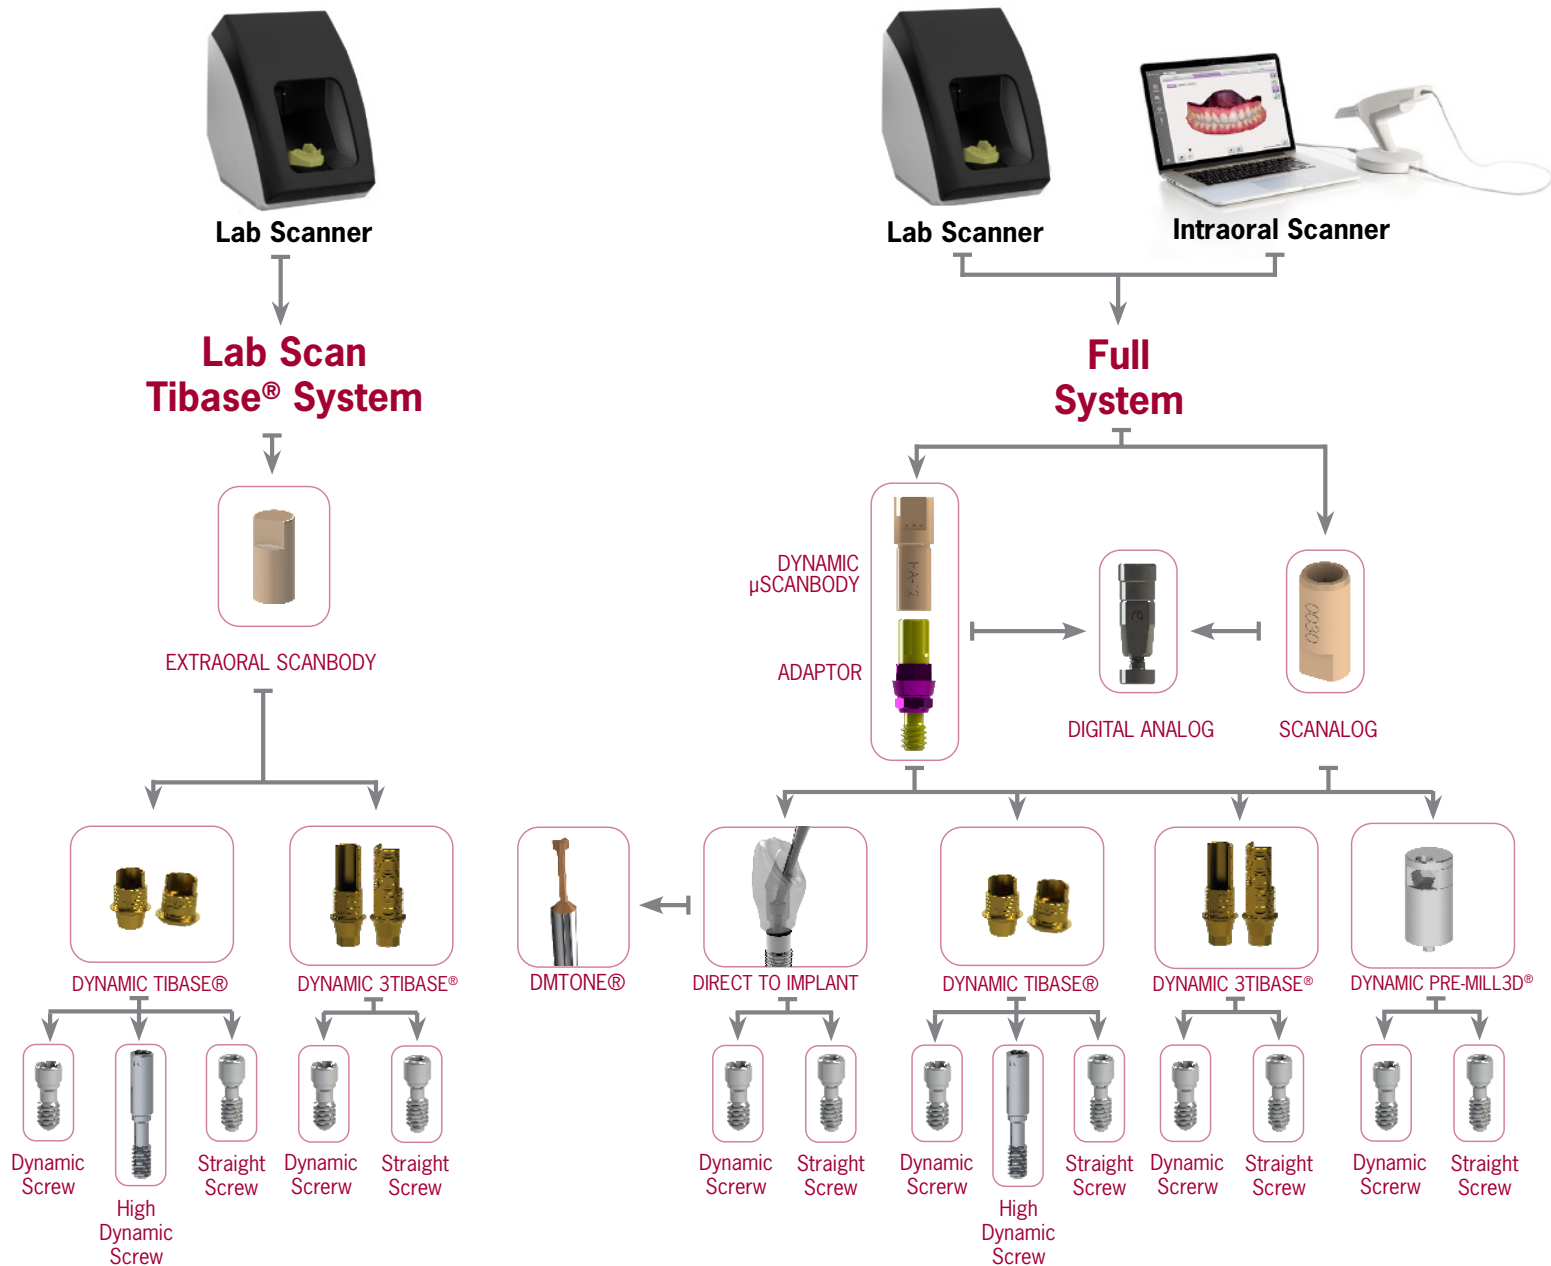

DYNAMIC SYSTEM for MILLING STRUCTURES

The Screwdriver set of 3.0 Dynamic Abutment® System is used in those cases in which rectification of the entry of the screw due to an unfavorable position of the implants is necessary, improving the functionality and aesthetics of the milled prosthesis.

More than 500.000 cases resolved with **DYNAMIC SYSTEM**



PATENT NUMBER
Dynamic Screwdriver
EP 3 260 079

Dynamic Screwdriver

Screwdriver with hexalobular head, exclusively to the 3.0 Dynamic Abutment® system.

Lengths: 18, 24, 32mm.



Our screwdriver has a contra-angle connection to make it easier to use with a dynamometer or manual ratchet, with the corresponding adaptors or handles.

Dynamic Screw

PATENT NUMBER
Dynamic Screw
US 2020/15942

High Dynamic Screw

Dynamic screws cover the majority of the thread metrics available on the market. They are used with the Dynamic TiBase® or milled structures with an angled screw channel. There are several lengths for each metric to ease adaptation to the structures.

All of them are made of Titanium grade V.

All screws are perfectly identified with their batch and reference numbers, which allow each and every screw to be traced and recorded in the patient's card and in the clinical or laboratory records. Only the 3.0 dynamic screwdriver must be used to install them.

DAS PRODUCTS

CAD-CAM WORKFLOW



DYNAMIC μSCANBODY

The scanbody detects the position and orientation of the respective dental implant or analog in CAD-CAM scanning procedures.


Hole free scanbody and not screwed

There are no holes in the upper section which means the Z axis is free to improve scanbody scanning.

The angulation of the chimney it goes always on the opposite side of the scanbody lateral cut.



3 lenghts
(8mm, 10mm and 12mm) for the most complex scanbody reading cases.

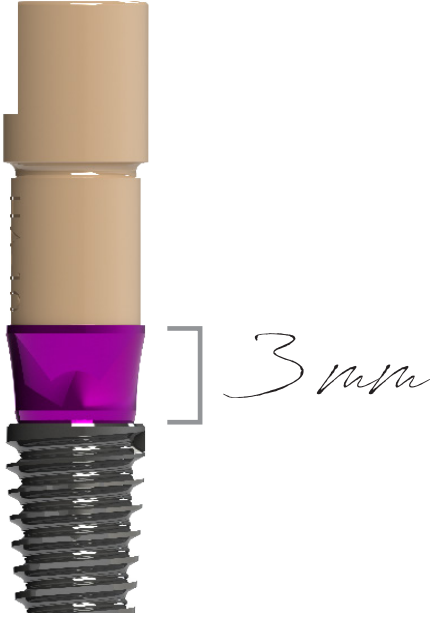


ADAPTOR

Fastened to an adaptor using a magnet

Connecting element between the scanbody and the implant. Marked with different colors according to the compatibility*


*See pages 176 to 179

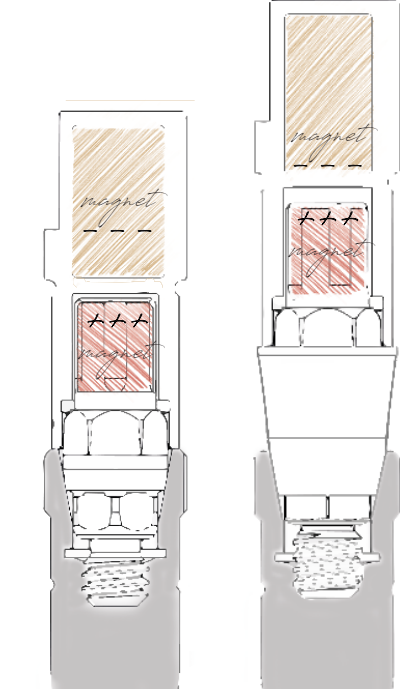

OPTION 1
library
DAS_I_XXXX

OPTION 2
library*
DAS_IG_XXXX

*Use IG Library code with the 3mm adaptor

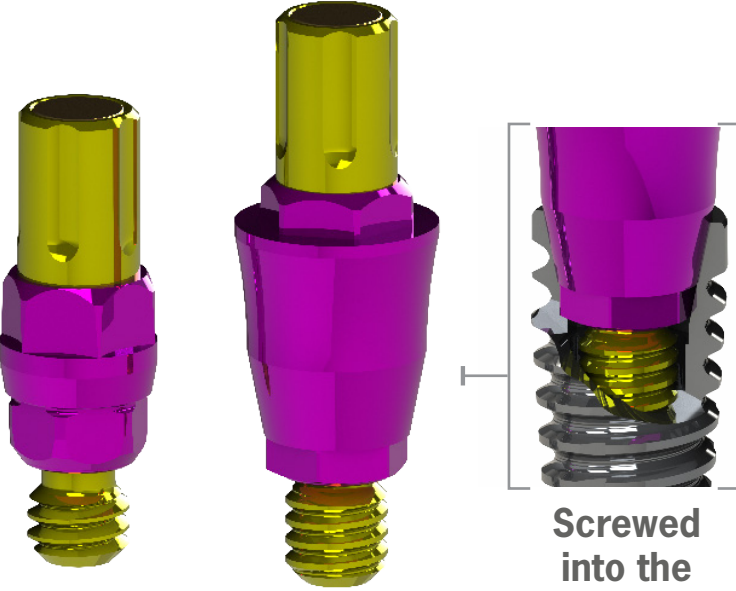


Screwed into the implant

Special screwdriver for the adaptor*
*See page 182





LAB SCANBODY

Only for Dynamic TiBase®
and Lab Scanner

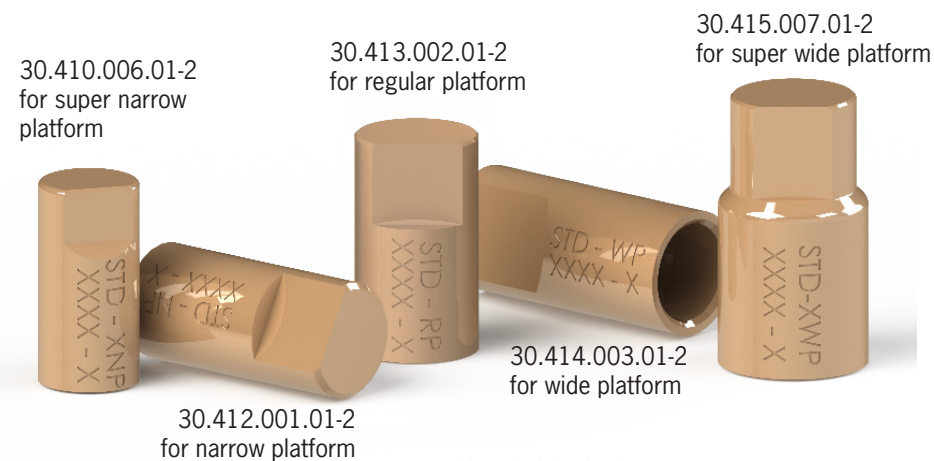


30.413.004.01-2
for compatibility 0037

Special
scanbodies

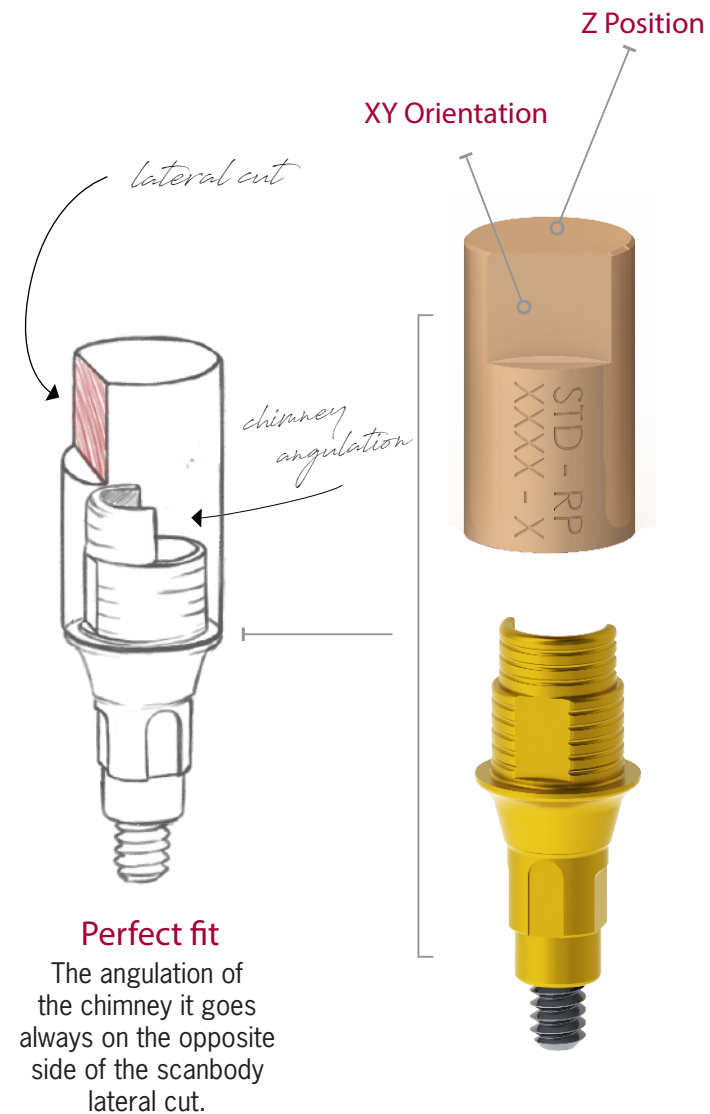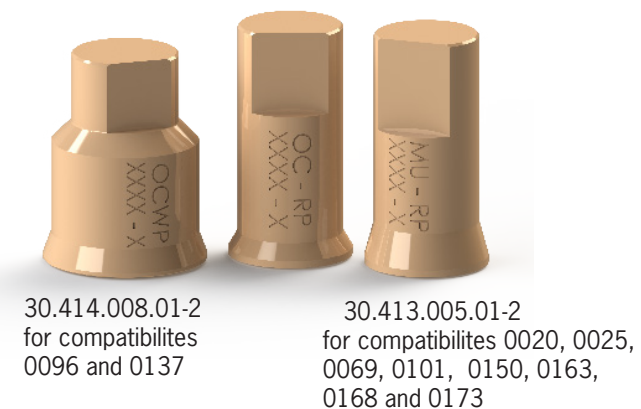

ScAnalog

Scan directly on the impresion tray

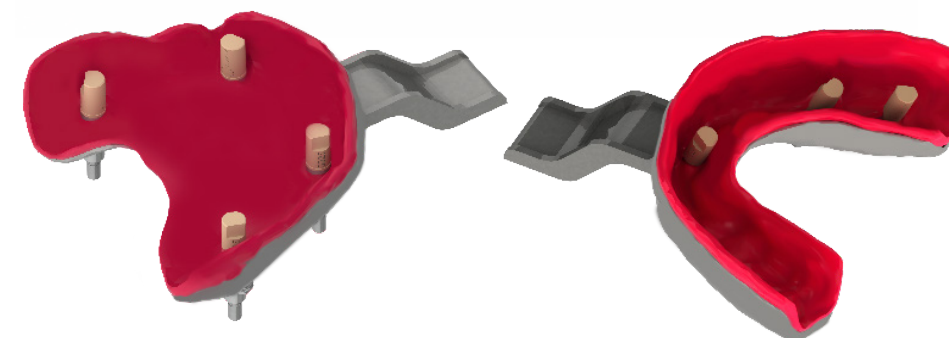

Scanning

Scanning process of the
silicon model with the
ScAnalog placed.

DYNAMIC TIBASE® *

Dynamic TiBases® are a technological contribution to the digital treatment for the angled systems development using CAD-CAM: the Dynamic System includes the Dynamic TiBase®, the dynamic screw-screwdriver set, scanbodies and digital libraries available for the main CAD softwares on the market: Exocad, 3Shape, Dentalwings and Dental Cad.

PATENT NUMBER
Dynamic TiBase®
US 10.130.447

TO CORRECT
ANGULATION

up to
45°




Dynamic
screw

Straight
screw


*Maximum angulation available for the first TiBase gingival height. Maximum angulations for the rest of gingival heights under development

Our grade V titanium bases are **gold anodized** to improve the work's aesthetic.

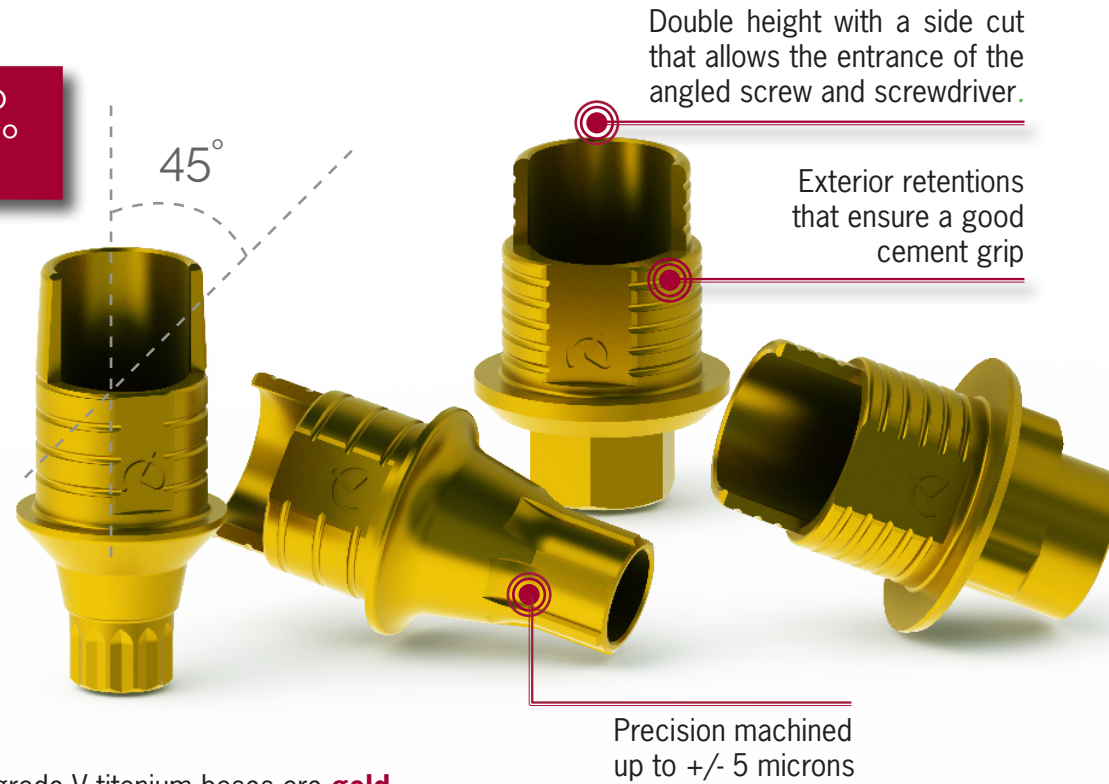

DYNAMIC 3TIBASE®

The Dynamic 3TiBase® offers the possibility to work with different cement heights: 5, 7 or 9mm. It is specially designed for the cases that require higher height. In this way, a greater support surface is achieved, the structure is stronger and more resistant so structure breaks by height decompensation between the TiBase and the structure are avoided.

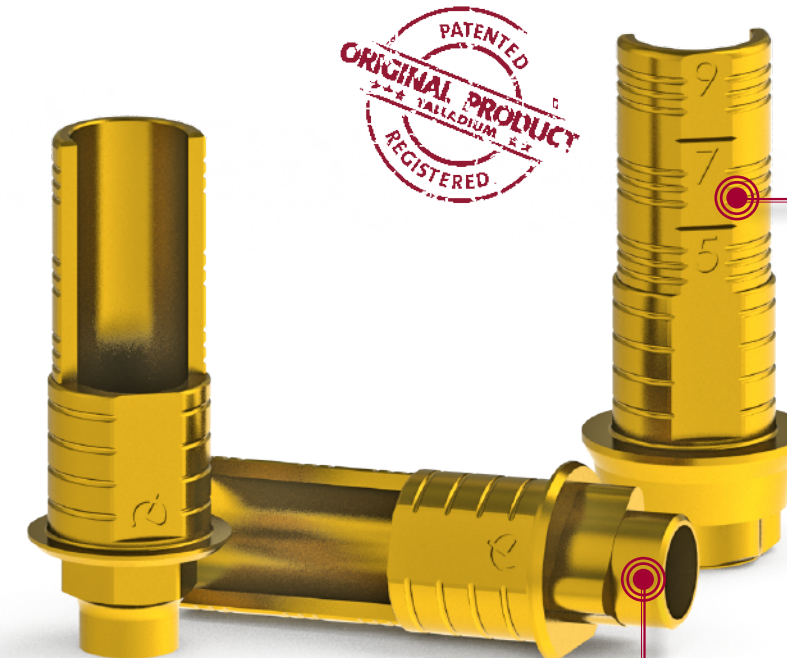

To achieve the maximum strength of the structure it is important to have the maximum support surface possible.

Precision machined up to +/- 5 microns




Scan with the Dynamic μScanbody and cement the final piece onto the 3TiBase.



If you do not have the Dynamic μScanbody, it is necessary to use the 4mm TiBase and the Lab scanbody to make the scanning. The final piece is cemented onto the 3TiBase.

DYNAMIC TIBASE®

Gingival options

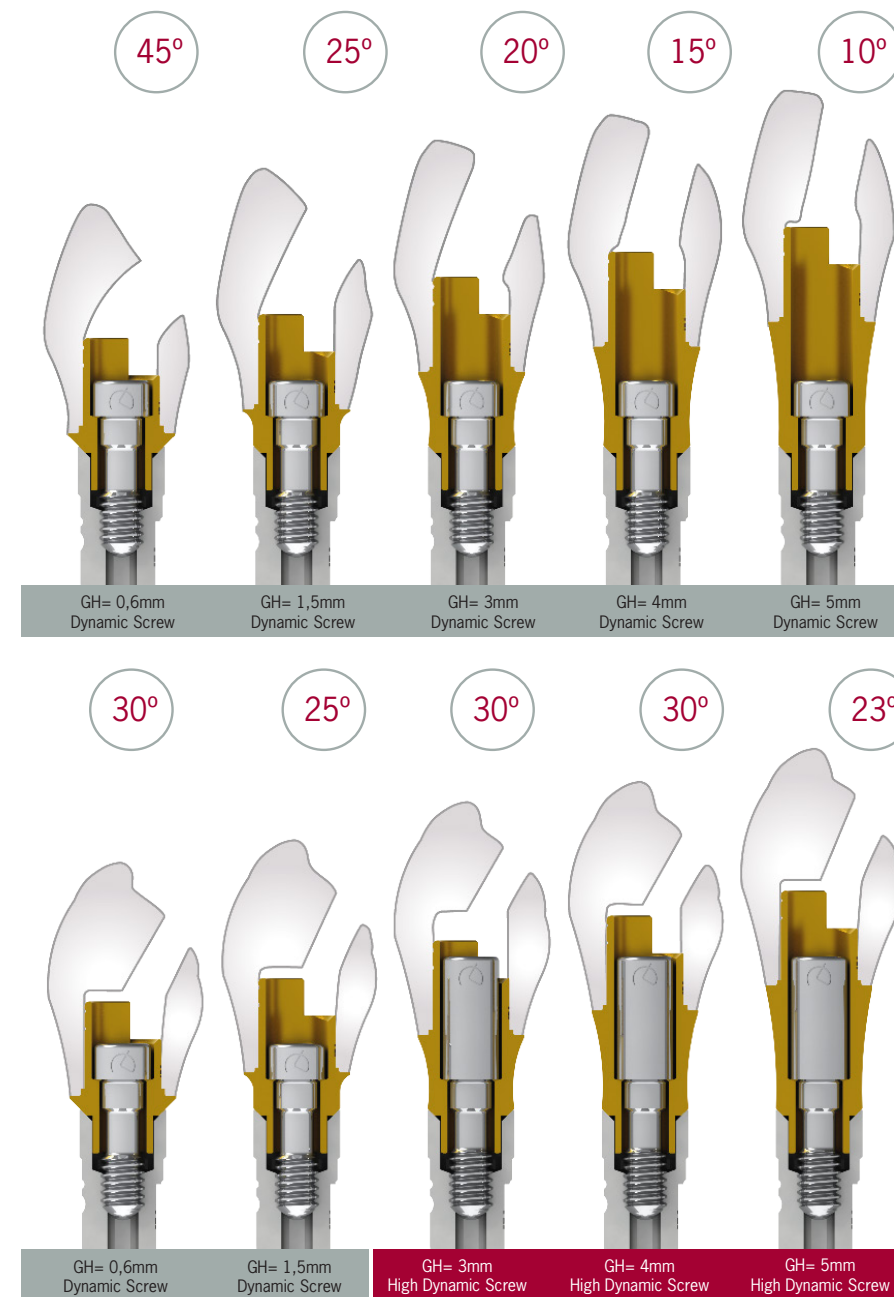


*Example with TiBase® compatible with Zimmer Screw-Vent Ø3,5 (Code 0040)



- Keep the angulation
 - Best aesthetic angled channel Ø 2mm
 - Angled channel reduction of 32%
 - Increases the volume of the structure
 - Captive Screw
- (Put the screw on the TiBase® before cementing)




DYNAMIC PRE-MILL3D®



Pre-milled angled channel

The Dynamic Premill3d® already comes with a pre-milling of the inner channel



Angulation from 0 to 30° choice

Allows to choose angulation of the screw channel on the CAD for the later insertion of the screw



Milling of the angulated screw channel


CAD design and milling of the angled channel on CAM by the customer



Dynamic Pre-milled final structure



Precision machined up to +/- 5 microns

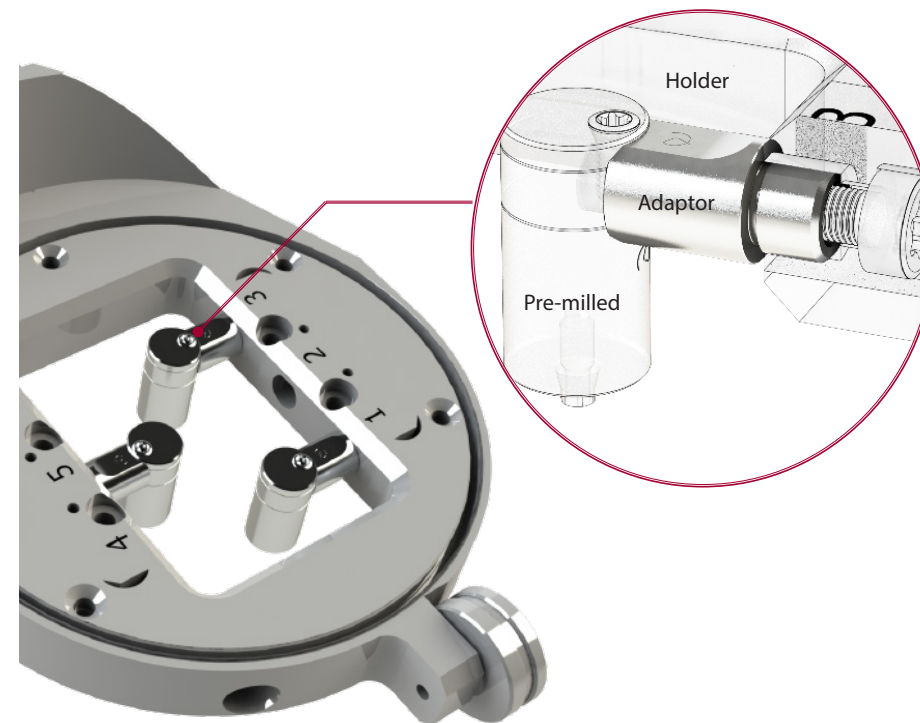


ADAPTORS



It is not necessary to purchase a new holder

The adapter has the holder connection and connects the holder to the pre-milled abutment.

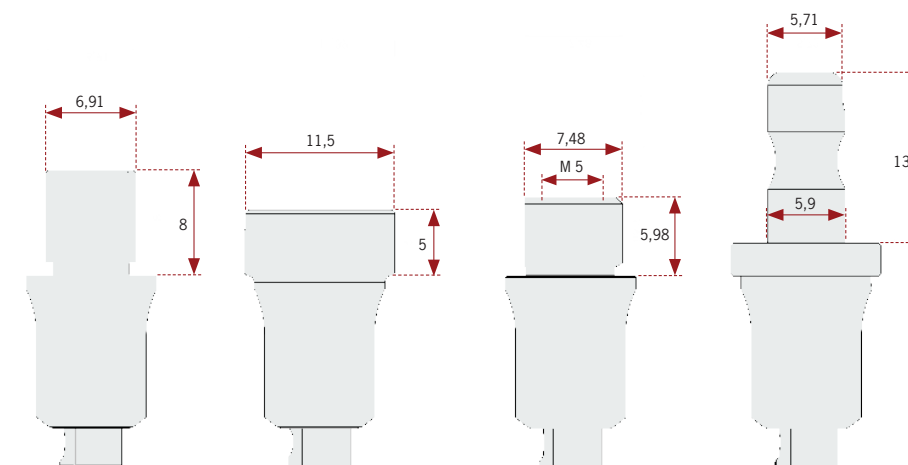

Customized ADAPTORS

We design and manufacture the adapter for any type of holder
(das@dynamicabutment.com)

DYNAMIC MILLING TOOL

Each tool is compatible depending on **screw seating, metric and length**

DIRECT TO IMPLANT (one piece) and ANGULATED

Precision milling tool. In the screwed angled structure direct to implant, it is used to mill the screw seating and to increase the internal diameter of the straight channel.

There are 3 cutting wing-tips with 3 different cutting area each, to mill the screw seating and to increase the internal diameter of the straight channel.


PATENT NUMBER
Milling process of the
angulated channel
ES 2658 985



STEP 1:
Crown with
pre drill.




STEP 2:
Crown with
Angled channel.

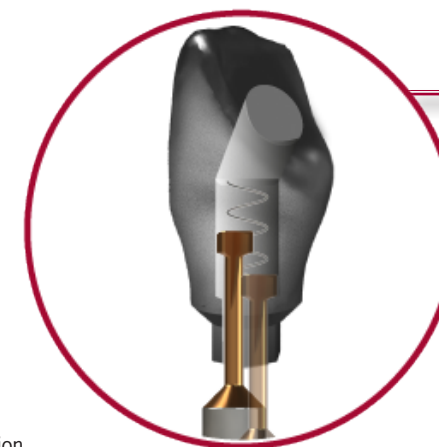



STEP 3:
Crown with Dynamic Milling
Tool.
Milling the screw seat and
increasing the diameter of
the straight channel.

*Direct to implant maximum angulation
under development

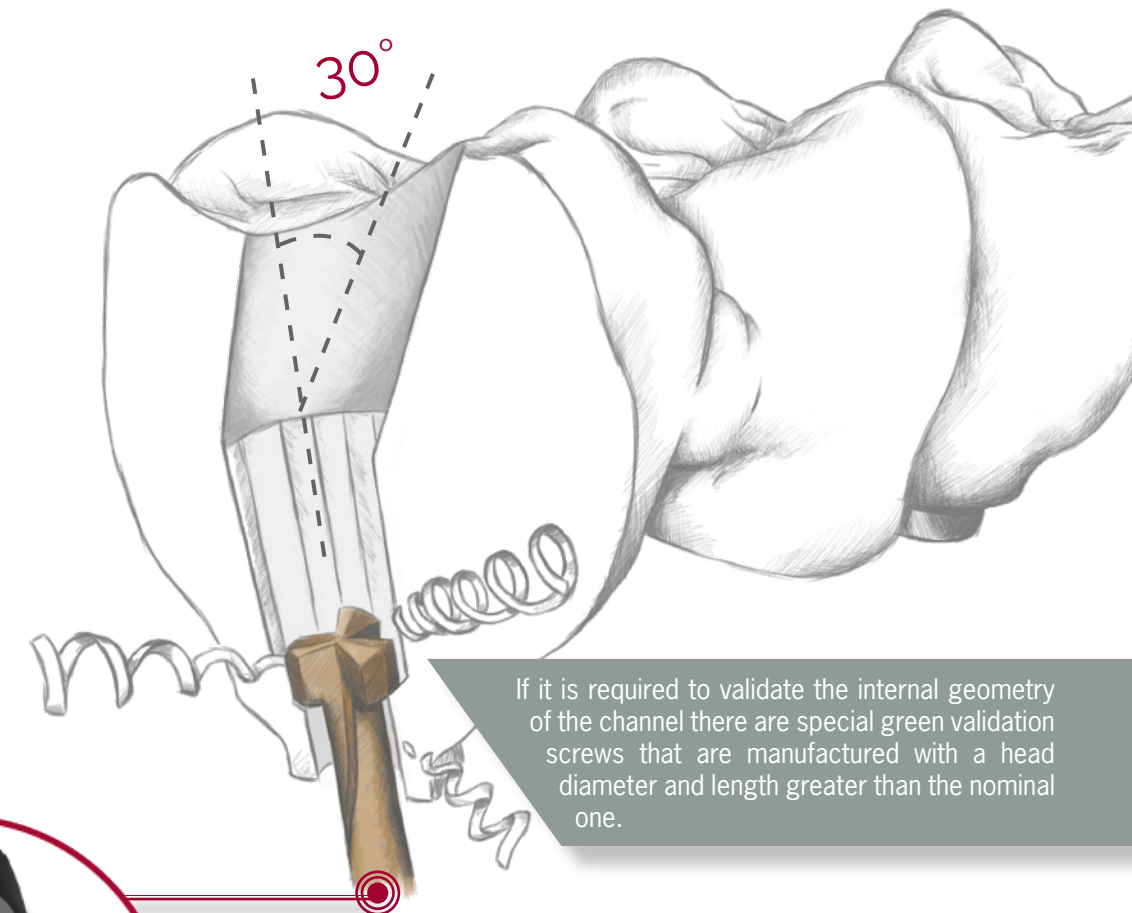


If it is required to validate the internal geometry of the channel there are special green validation screws that are manufactured with a head diameter and length greater than the nominal one.

**TESTED and
VALIDATED by**



DMTONE
DYNAMIC MILLING TOOL

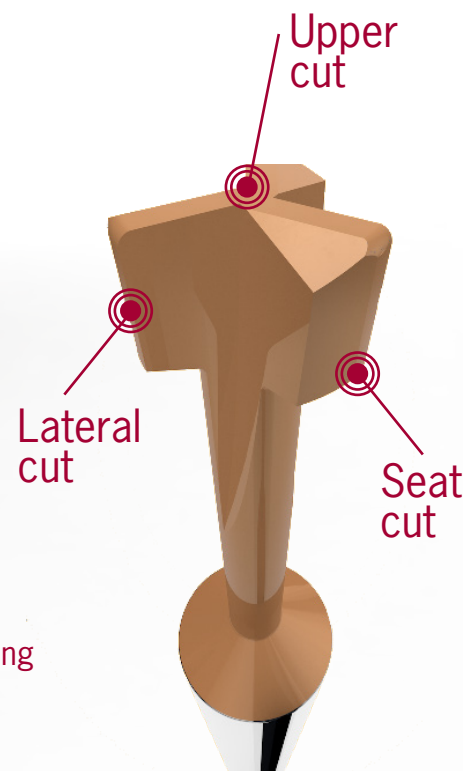

DIGITAL ANALOG

Digital analog of the dental implant to simulate implant position in a 3D printed dental model.




3D PRINTED MODEL


The dental model - for later insertion of the analogs - is designed using the CAD libraries.



3shape
Model Builder




exocad
Model Creator




dental wings
Model Builder


Concave notch
Top precision in longitudinal position



Curved Surface
Accuracy of orientation guaranteed





Longitudinal cut
Longitudinal cut to avoid rotation X-Y



Screwed fastening
Prevents the analog from moving in Z



DAS LIBRARIES

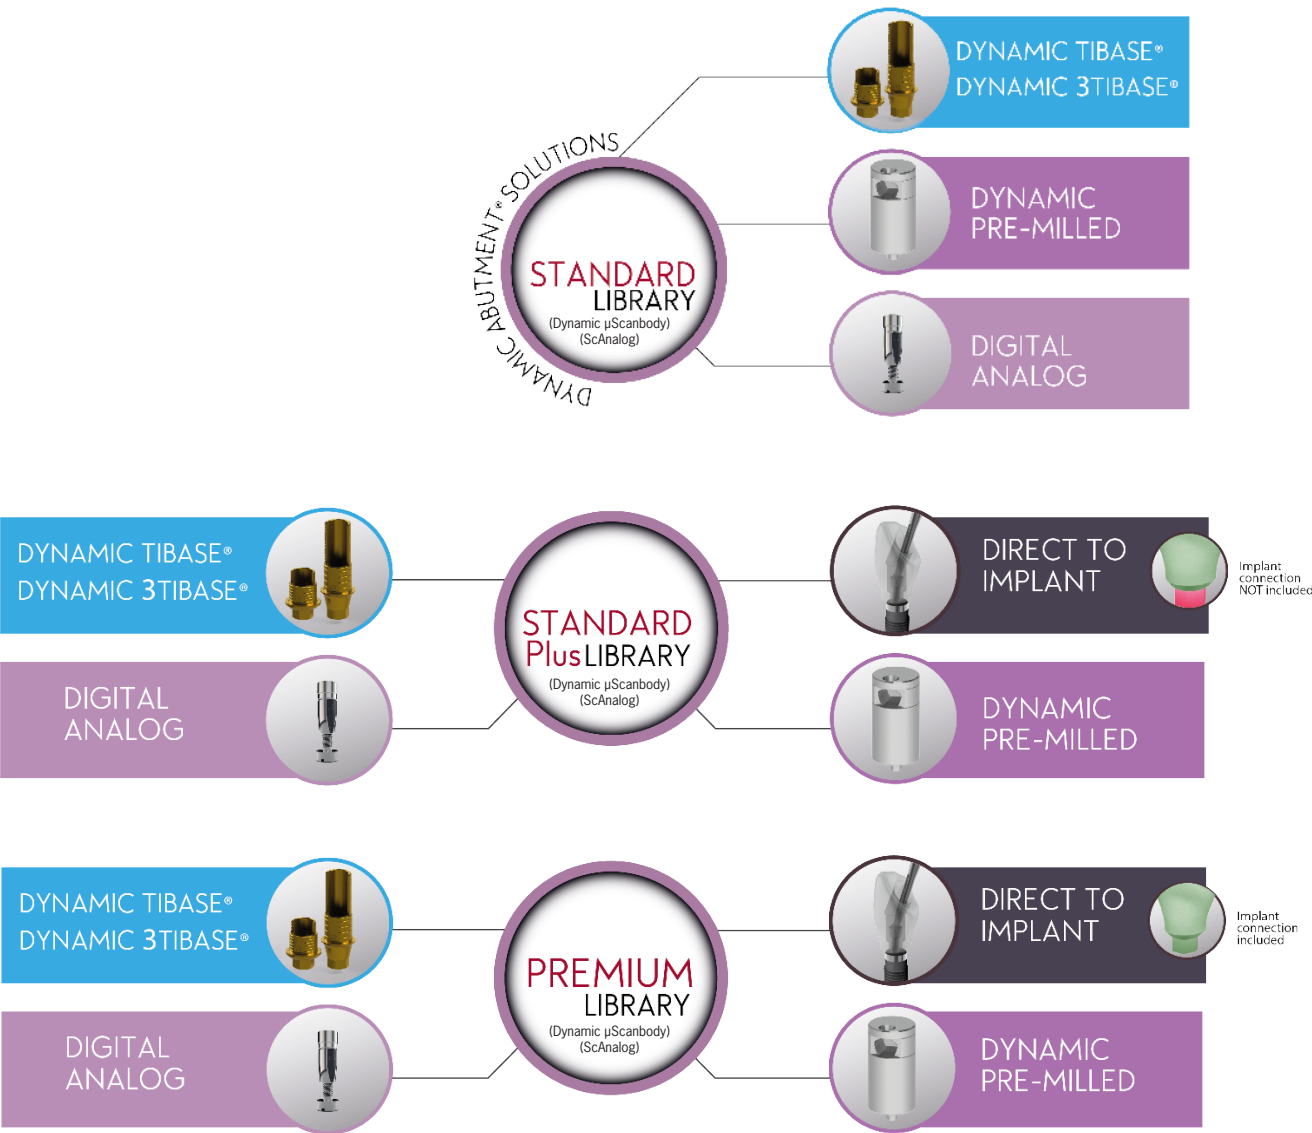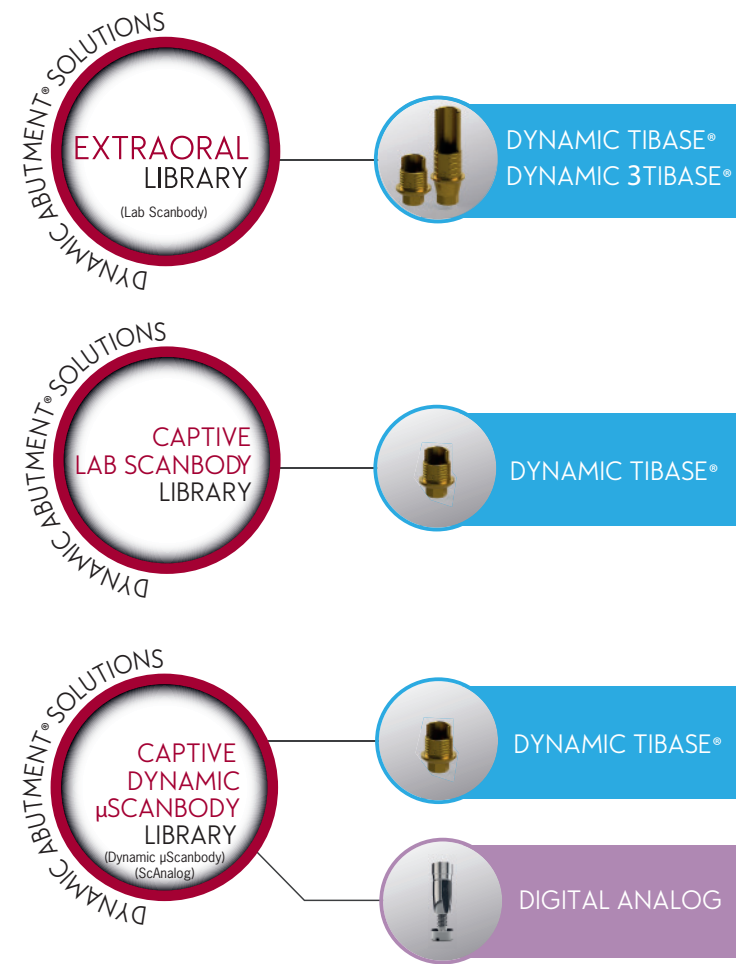


YOUR DIGITAL DENTAL PARTNER

DAS customize services

PRODUCT DEVELOPMENT


Any DAS traded goods can be made-to-measure or adapted to your work protocol. DAS complements the development of new products with the technological support (software, libraries, tools, etc.) necessary, alongside all the guarantees any healthcare product needs.

CAD ADAPTION SERVICES

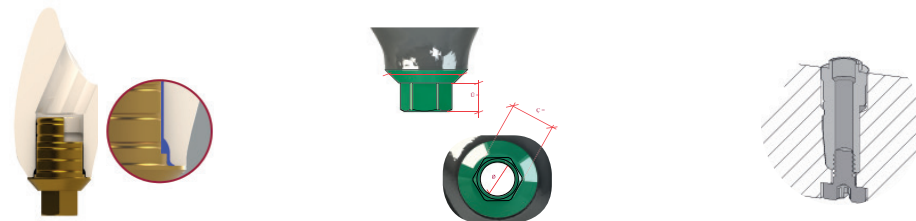

- ✳ Adjustment of the CAD libraries for our products to client needs: angled channel diameter modification, calibration of cemented gap TiBase®, adjustment of 3D digital analog printing gap, etc.
- ✳ CAD libraries supplied with implant connections; DAS currently has over 500 implant compatibilities.
- ✳ Development of special CAD libraries for connections pertaining to the client.
- ✳ Design of libraries linked to client's specific scanbodies.
- ✳ Etc.

CAM SUPPORT and ADVICE

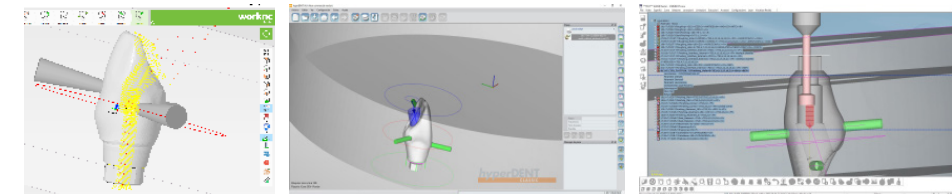

Dynamic Abutment® Solutions products have been tested and validated by the leading CAM software brands on the market.

- ✳ Provision of implant connections with nominal values.
- ✳ Design and production of special tools to mill connections or special geometries (abutments).
- ✳ Design and production of special supports for your milling equipment: pre-milled supports, etc.
- ✳ Technology for machining angled channels (copyright-free).



SPECIALIZED CONSULTANCY



Multidisciplinary experience in different areas of dental research and regular collaboration on projects with the key operators in the sector have provided us with experience and know-how that we want to make available to you, so we can advise you, work together and pursue customized projects. All DAS technological and human resources are available to help turn your idea into a reality, providing expert advice and support throughout all the developmental stages.

DYNAMIC TIBASE®

CAD

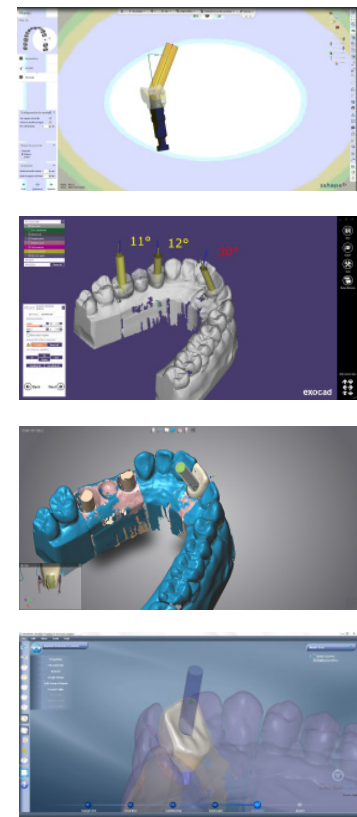


3shape

exocad

dental wings

DentalCad

CAM

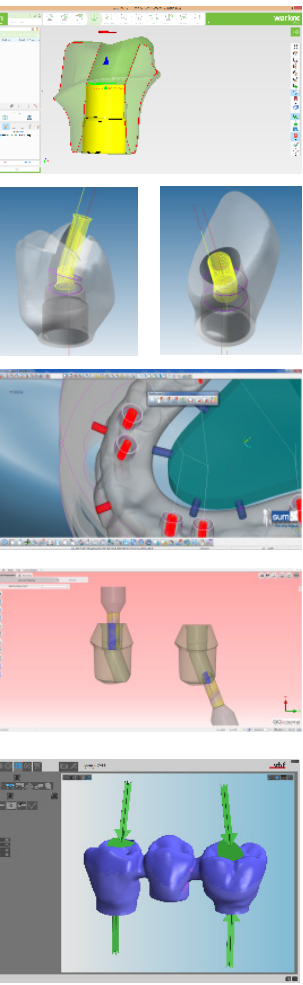

Tested CAM Software

worknc Dental


FOLLOW-ME! TECHNOLOGY GROUP

MILL BOX sum


GO2dental cam for dental labs

vhf

DIRECT to IMPLANT

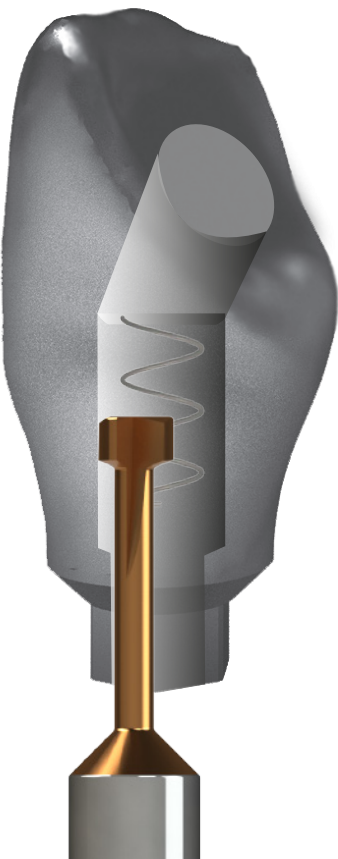

CAD

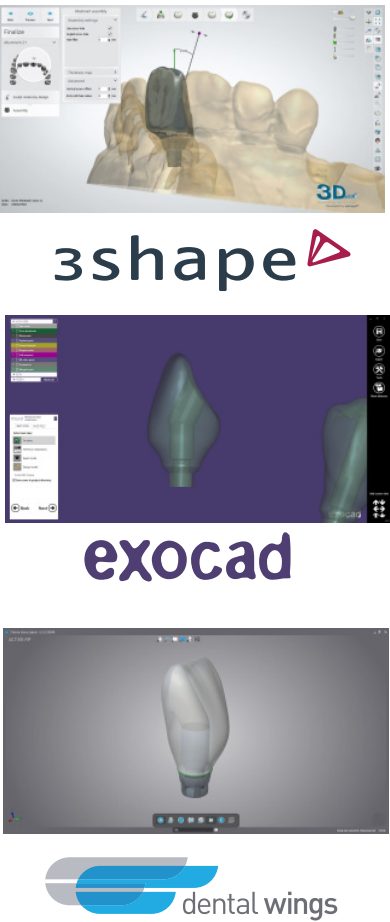

3shape

exocad

dental wings

CAM



worknc Dental

FOLLOW-ME! TECHNOLOGY GROUP

MILL BOX sum


DIGITAL ANALOG




CAD-CAM



3shape
Model Builder

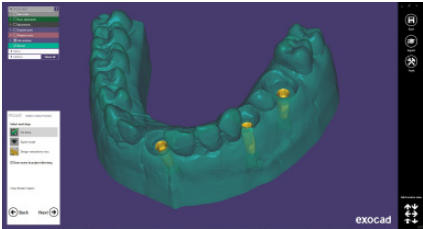

exocad
Model Creator

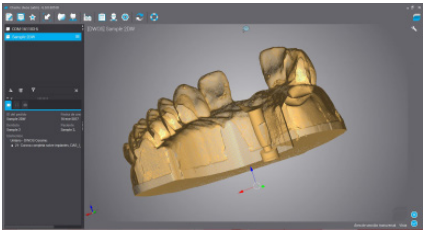


dental wings
Model Builder


DYNAMIC PRE-MILL3D®




CAD

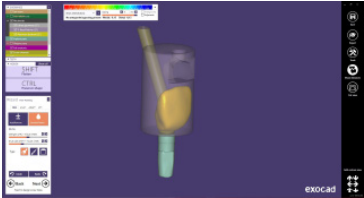

exocad

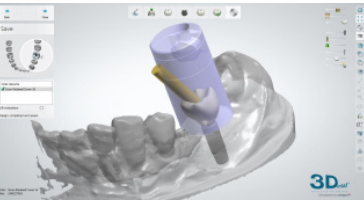


3shape




dental wings

CAM

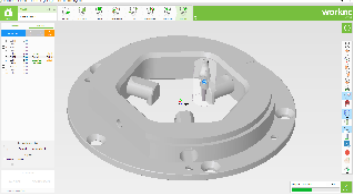

worknc
Dental

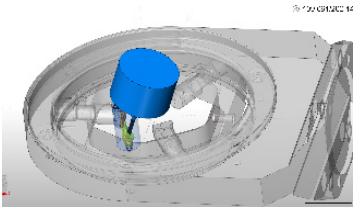


MILL BOX
sum

FOLLOW-ME!
TECHNOLOGY GROUP

*Soon

DYNAMIC SYSTEM

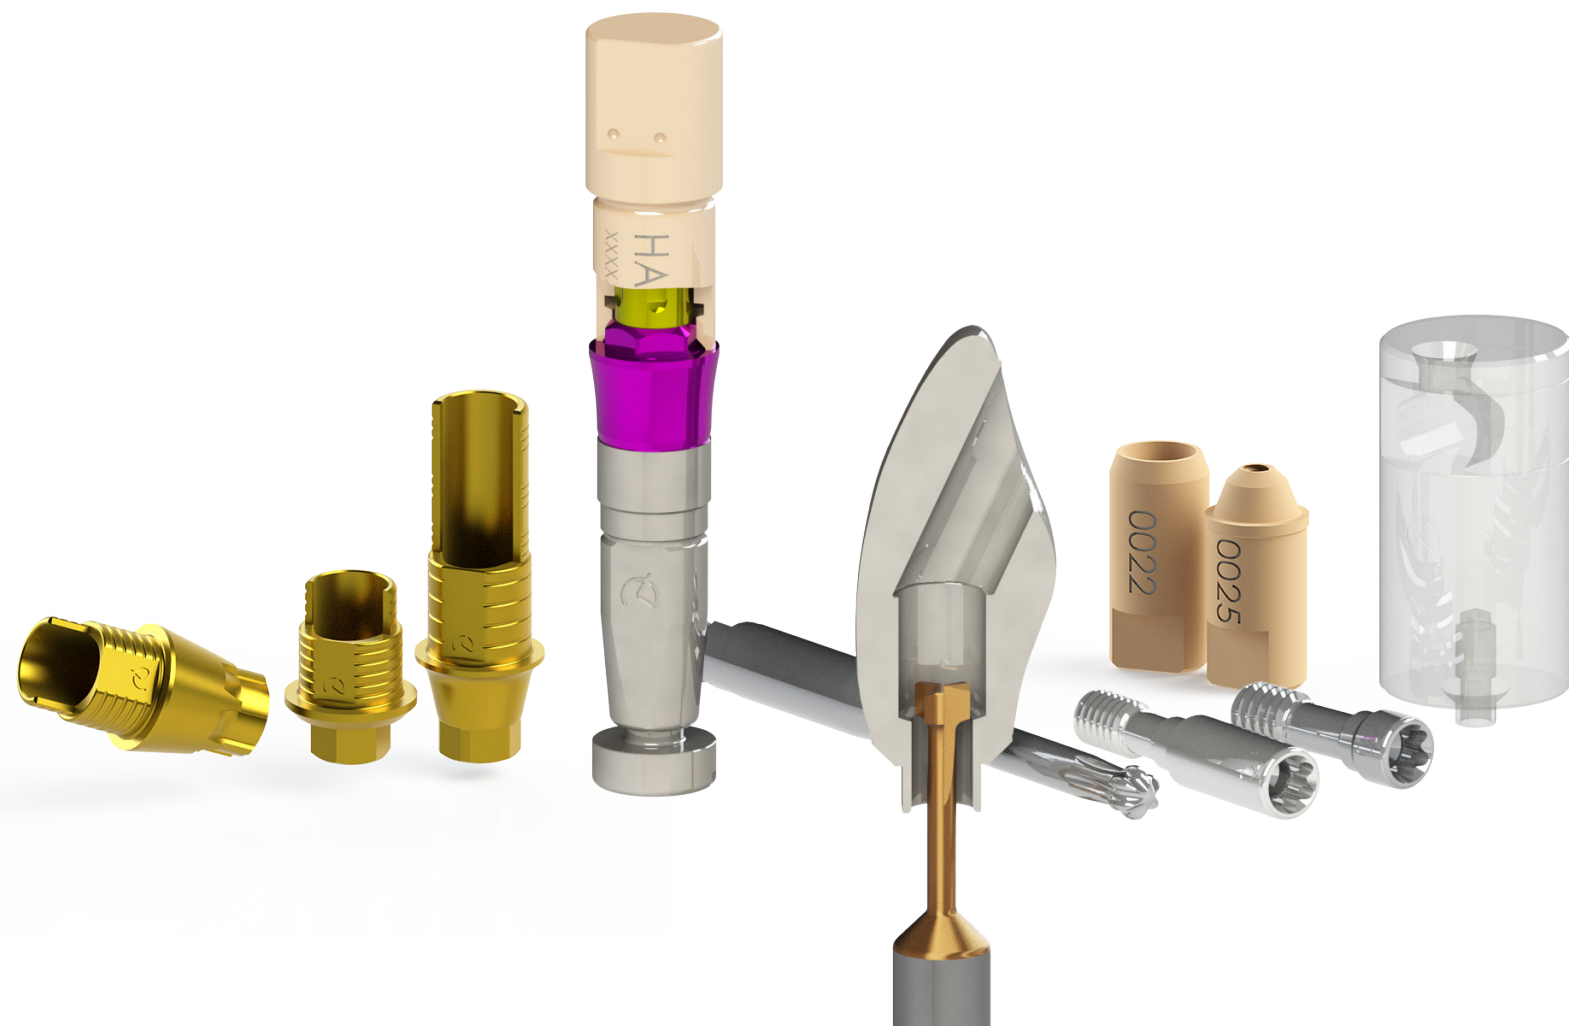

List of compatibilities available

AB
ACE
ADIN
ALPHABIO
ANCLADEN
ANKYLOS
ANTHOGRYR
ARDS
ASTRA
AVINENT
BEGO
BIOCONCEPT
BIOGENESIS
BIOHORIZONS
BIOMET 3i
BIOLOK
BIONER
BIOTEC
BIOTECH
BREDENT MEDICAL
BTI
BTK
B&W
CAMLOG
CONEXÃO SISTEMA DE PRÓTESE
CORTEX
DENTAL TECH
DENTAURUM
DENTIS
DENTIUM

DIO IMPLANTS
EASY IMPLANT
ECKERMANN
ELITE MEDICA
EUROTEKNIKA
GALIMPLANT
GC TECH
GLOBAL D (TEKKA)
GMI (ILERIMPLANT)
GT MEDICAL
HAHN IMPLANT (GLIDEWELL)
HI-TEC
HIOSSEN
IBS
IDO IMPLANTS
IHDE DENTAL (IMBIODENT)
IMPLANT DIRECT
IMPLANT GENESIS
INTRA-LOCK
JDENTALCARE
KEystone
KLOCKNER
LASAK
LEADER
MEDENTIS
MEGAGEN
MICRODENT
MIS
MOZO-GRAU
MPI

NEOBIOTECH
NEODENT
NEOSS
NOBEL BIO CARE
NORIS MEDICAL
NORMON
NOVA IMPLANTS
OSSTEM IMPLANT
OSTEOPLUS
PALTOP
PHIBO
PROCLINIC
RADHEX
SEWON MEDIX
SGS
SIC INVENT
SIGNO VINCES
SOUTHERN IMPLANTS
STRAUMANN
SYBRON IMPLANT SOLUTIONS
TITANIUM - FIX
TRE-OSS
TRI DENTAL IMPLANTS
TRINON
UFIT
VULKAN IMPLANTS
XIVE
YES IMPLANT
ZIACOM (OSSEOLIFE)
ZIMMER

AB

✿ I2	Implant: Ø 3,5/3,75/4,2/4,5/ 5/6 Platform: Standard (Code 0040)	p. 87
✿ I22	Implant: Ø 3,75/4,22 Platform: Standard (Code 0040)	p. 87
✿ I5	Implant: Ø 3,5/3,75/4,2/4,5/5/6/7/8 Platform: Standard (Code 0040)	p. 87
✿ I55	Implant: Ø 3,75/4,2/4,5/5/6/7/8 Platform: Standard (Code 0040)	p. 87
✿ I10	Implant: Ø 4,2/5 Platform: Standard (Code 0040)	p. 87
✿ I15	Implant: Ø 6/7/8 Platform: Standard (Code 0040)	p. 87
✿ Multi Unit D1-P64	Platform: Universal (Code 0025)	p. 76

ACE

✿ External Hex	Implant: Ø 3,3 Platform: NP 3,5 (Code 0023)	p. 74
	Implant: Ø 3,75/4 Platform: RP 4,1 (Code 0024)	p. 75
	Implant: Ø 4,75 Platform: WP 5 (Code 0058)	p. 102

✿ Infinity TRI-CAM	Implant: Ø 3,5 Platform: 3,5 (Code 0026)	p. 77
	Implant: Ø 4,3 Platform: 4,3 (Code 0027)	p. 78
	Implant: Ø 5 Platform: 5 (Code 0028)	p. 79
✿ Infinity Internal Hex	Implant: Ø 3,7/4,1 Platform: 3,5 (Code 0040)	p. 87
	Implant: Ø 4,7/5,1 Platform: 4,5 (Code 0041)	p. 89
✿ Infinity Octagon	Implant: Ø 3,3/4,1/4,8 Platform: RP 4,8 (Code 0037)	p. 84
	Implant: Ø 4,8 Platform: WP 6,5 (Code 0096)	p. 119
✿ Multi Unit	Platform: Universal (Code 0025)	p. 76

ADIN

✿ Swell	Implant: Ø 3,3 Platform: 3,45 (Code 0040)	p. 87
	Implant: Ø 3,75/4,2 Platform: 3,6 (Code 0040)	p. 87
	Implant: Ø 5 Platform: 4 (Code 0040)	p. 87
	Implant: Ø 6 Platform: 4,6 (Code 0040)	p. 87

✿ Touareg-S / Touareg-OS	Implant: Ø 3,5 Platform: 3,45 (Code 0040)	p. 87
	Implant: Ø 3,75/4,2 Platform: 3,6 (Code 0040)	p. 87
	Implant: Ø 5 Platform: 4 (Code 0040)	p. 87
	Implant: Ø 6 Platform: 5 (Code 0040)	p. 87
✿ Touareg CloseFit	Implant: Ø 3,5 Platform: RP (Code 0021)	p. 72
	Implant: Ø 4,3/5 Platform: WP (Code 0022)	p. 73
✿ Multi Unit TMA	Platform: Universal (Code 0025)	p. 76

ALPHABIO

✿ Internal Hex Connection (IH) SPI	Implant: Ø 3,3/3,75/4,2/5/6 Platform: Universal (Code 0040)	p. 87
✿ Internal Hex Connection (IH) ICE	Implant: Ø 3,7/3,75/4,2/4,65/5,3 Platform: Universal (Code 0040)	p. 87
✿ Internal Hex Connection (IH) DFI	Implant: Ø 3,3/3,75/4,2/4,5 Platform: Universal (Code 0040)	p. 87
✿ Internal Hex Connection (IH) ATID	Implant: Ø 3,3/3,75/4,2/5/6 Platform: Universal (Code 0040)	p. 87
✿ Internal Hex Connection (IH) NEO	Implant: Ø 3,75/4,2/5 Platform: 3,5 (Code 0040)	p. 87

✿ Conical Hex Connection (CHC) NICE	Implant: Ø 3,2 Platform: Narrow (Code 0136)	p. 135
✿ Conical Hex Connection (CHC) NEO	Implant: Ø 3,2/3,5 Platform: Narrow (Code 0136)	p. 135
✿ Conical Standard Connection (CS)	Implant: Ø 3,75/4,2/5 Platform: Standard (Code 0169)	p. 151

ANCLADEN

✿ Anclalink	Implant: Ø 3,75/4,25/5 Platform: 3,5 (Code 0040)	p. 87
-------------	---	-------

ANKYLOS

✿ Ankylos	Implant: Ø 3,5 Platform: 3,5 (Code 0075)	p. 108
	Implant: Ø 4,5 Platform: 4,5 (Code 0075)	p. 108
	Implant: Ø 5,5 Platform: 5,5 (Code 0075)	p. 108
	Implant: Ø 7 Platform: 7 (Code 0075)	p. 108

ANTHOGRY

✿ Axiom REG / PX	Implant: Ø 3,4 Platform: 3,4 (Code 0161)	p. 143
	Implant: Ø 4 Platform: 4 (Code 0149)	p. 137
	Implant: Ø 4,6 Platform: 4,6 (Code 0149)	p. 137
	Implant: Ø 5,2 Platform: 5,2 (Code 0162)	p. 144

✿ Anthofit HE	Implant: Ø 5 Platform: L (5) (Code 0058)	p. 102
✿ Ossfit	Implant: Ø 3,5/4,2 Platform: 4,8 (Code 0074)	p. 107
	Implant: Ø 3,5/4,2 Platform: 4,8 (Code 0037)	p. 84
	Implant: Ø 5 Platform: 6,5 (Code 0096)	p. 119
✿ Multi Unit	Implant: Ø 4,8 Platform: Universal (Code 0163)	p. 145

ARDS

✿ Smart	Implant: Ø 3,75/4,2/4,5 Platform: 3,75 (Code 0040)	p. 87
✿ Classic	Implant: Ø 3,75/4,2/4,5 Platform: 3,75 (Code 0040)	p. 87
	Implant: Ø 3,3/3,75/4,2/5/6 Platform: 3,75 (Code 0040)	p. 87
✿ Premium	Implant: Ø 3,3/3,75/4,2/5/6 Platform: 3,75 (Code 0040)	p. 87

✿ CIT	Implant: Ø 3,3/3,75/4,2/5/6 Platform: 3,75 (Code 0040)	p. 87
-------	---	-------

ASTRA

✿ Yellow	Implant: Ø 3 Platform: Yellow (Code 0109)	p. 122
✿ Aqua	Implant: Ø 3,5/4 Platform: Aqua (Code 0004)	p. 55
✿ Lilac	Implant: Ø 4,5/5 Platform: Lilac (Code 0005)	p. 56
✿ Cono 20°	Platform: Regular/Wide (Code 0066)	p. 106
✿ Evolution (Internal)	Implant: Ø 3 Platform: 3.0 (Code 0090)	p. 116
	Implant: Ø 3,6 Platform: 3.6 (Code 0006)	p. 57
	Implant: Ø 4,2 Platform: 4.2 (Code 0007)	p. 58
	Implant: Ø 4,8 Platform: 4.8 (Code 0091)	p. 117
	Implant: Ø 5,4 Platform: 5.4 (Code 0092)	p. 118
✿ Uni Abutment	Platform: Universal (Code 0008)	p. 59

AVINENT

✿ HE/EC	
Implant: Ø 3,3/3,8/4/4,2/4,8//4,5/5	
Platform: 4,1 (Code 0024)	p. 75
Implant: Ø 4,8	
Platform: 5,1 (Code 0061)	p. 105
✿ HI/IC	
Implant: Ø 3,1//3,5/4	
Platform: 3,5 (Code 0040)	p. 87
Implant: Ø 3,3/3,8/4/4,2/4,8//4,5/5	
Platform: 4,1 (Code 0040)	p. 87
✿ Transepitelial	
Platform: Regular (Code 0025)	p. 76

BEGO

✿ RS/RSX	
Implant: Ø 3.0	
Platform: 3.0 (Code 0049)	p.96
✿ S/RI/RS/RSX	
Implant: Ø 3,25/3,75	
Platform: 3,67 (Code 0050)	p. 97
Implant: Ø 4,1	
Platform: 4,1 (Code 0051)	p. 98
Implant: Ø 4,5	
Platform: 4,5 (Code 0052)	p. 99
Implant: Ø 5,5	
Platform: 5,5 (Code 0081)	p. 110
✿ MINI	
Implant: Ø 2,7/2,9/3,1	
Platform: Mini (Code 0187)	p.157
✿ MULTIPLUS	
Platform: Universal (Code 0150)	p.138

BIOCONCEPT

✿ BC Tissue Level Standard	
Implant: Ø 3,3/4,1/4,8	
Platform: Regular (Code 0037)	p. 84
✿ BC Tissue Level Standard Plus	
Implant: Ø 4,8	
Platform: Regular (Code 0037)	p. 84
✿ BC Tissue Level Tapered Effect	
Implant: Ø 4,8	
Platform: Regular (Code 0037)	p. 84
✿ BC Bone Level	
Implant: Ø 3,3	
Platform: Narrow (Code 0033)	p. 82
Implant: Ø 4,1/4,8	
Platform: Regular (Code 0035)	p. 83
✿ BV Tapered Bone Level	
Implant: Ø 3,5	
Platform: Narrow (Code 0029)	p. 80
Implant: Ø 4/4,5/5	
Platform: Regular (Code 0030)	p. 81

BIOGENESIS

✿ 3icon	
Implant: Ø 3,3	
Platform: Mini (Pink) (Code 0023)	p. 74
Implant: Ø 3,75/4/4,3/4,5	
Platform: Regular (Blue) (Code 0024)	p. 75
Implant: Ø 5/5,5	
Platform: Wide (Yellow) (Code 0058)	p. 102
✿ Aticon	
Implant: Ø 3,5/4/4,5/5	
Platform: Blue (Code 0005)	p. 56
✿ Aticon (Cone 20°)	
Platform: Regular/Wide (Code 0066)	p. 106

✿ Iticon	
Implant: Ø 3,5/4,1/4,8	
Platform: 4,8 (Code 0037)	p. 84

BIOHORIZONS

✿ Tapered Internal	
Implant: Ø 3/3,4	
Platform: 3 (Grey) (Code 0102)	p. 121
Implant: Ø 3,8	
Platform: 3,5 (Yellow) (Code 0040)	p. 87
Implant: Ø 4,6	
Platform: 4,5 (Green) (Code 0041)	p. 89
Implant: Ø 5,8	
Platform: 5,7 (Blue) (Code 0080)	p. 109

✿ Internal	
Implant: Ø 3,5/4	
Platform: 3,5 (Yellow) (Code 0040)	p. 87
Implant: Ø 4/5	
Platform: 4,5 (Green) (Code 0041)	p. 89
Implant: Ø 5/6	
Platform: 5,7 (Blue) (Code 0080)	p. 109

✿ Multi Unit	
Platform: Universal (Code 0025)	p. 76

BIOMET 3i

✿ Osseotite	
Implant: Ø 3,25	
Platform: 3,4 (Code 0003)	p. 54
Implant: Ø 3,75/4	
Platform: 4,1 (Code 0024)	p. 75

✿ Certain	
Implant: Ø 3,25/4	
Platform: 3,4 (Code 0001)	p. 52
Implant: Ø 4/5	
Platform: 4,1 (Code 0002)	p. 53
Implant: Ø 5	
Platform: 5 (Code 0057)	p. 101
✿ Low Profile	
Platform: Universal (Code 0025)	p. 76

BIOLOK

✿ External Hexagon	
Implant: Ø 3,45	
Platform: 3,45 (Code 0003)	p. 54

BIONER

✿ Ikelt / Bikelt	
Implant: Ø 3,3/3,75/4	
Platform: 4,1 (Code 0024)	p. 75

✿ Ikelt	
Implant: Ø 5	
Platform: 5 (Code 0058)	p. 102

✿ Hikelt	
Implant: Ø 3,8	
Platform: 3,95 (Code 0040)	p. 87
Implant: Ø 4,7	
Platform: 4,9 (Code 0041)	p. 89

✿ TopDM	
Implant: Ø 3,5	
Platform: 3,5 (Code 0021)	p. 72
Implant: Ø 4	
Platform: 4 (Code 0021)	p. 72
Implant: Ø 5	
Platform: 5 (Code 0021)	p. 72

✿ Transepitelial A-5M	
Platform: Regular (Code 0025)	p. 76

BIOTEC

✿ SPR/CIM	
Implant: Ø 3,3	
Platform: 3,3 (Code 0040)	p. 87
Implant: Ø 3,75	
Platform: 3,75 (Code 0040)	p. 87
✿ SPR/SPTT/CIM	
Implant: Ø 4,2	
Platform: 4,2 (Code 0040)	p. 87
Implant: Ø 5	
Platform: 5 (Code 0040)	p. 87

BIOTECH

✿ Kontakt	
Implant: Ø 3	
Platform: Yellow Narrow (Code 0164)	p. 146
Implant: Ø 3,6/4,2/4,8/5,4	
Platform: Regular (Code 0165)	p. 147

BREDENT MEDICAL

✿ Narrow Sky	
Implant: Ø 3,5	
Platform: NP 3,5 (Code 0110)	p. 123
✿ Blue Sky	
Implant: Ø 3,5/4/4,5/5,5	
Platform: 4 (Code 0111)	p. 124
✿ Blue Sky Classic	
Implant: Ø 3,5/4/4,5	
Platform: 4 (Code 0111)	p. 124

BTI

✿ External Connection Tiny	
Implant: Ø 2,5/3/3,3/3,5/3,75	
Platform: Tiny 3,5 (Code 0009)	p. 60

✿ ExternalConnection	
Implant: Ø 3,75/4/4,5/5	
Platform: Universal 4,1 (Code 0024)	p. 75
Implant: Ø 4,5/5/5,5	
Platform: Ancha 5,5 (Code 0060)	p. 104

✿ InternalConnection	
Implant: Ø 3,3/3,5/3,75/4/4,25/4,5/5/5,5	
Platform: Universal 4,1 (Code 0010)	p. 61
Implant: Ø 5/5,5/6/6,25	
Platform: Ancha 5,5 (Code 0059)	p. 103

✿ Multi-IM	
Platform Universal 4,1 (Code 0151)	p. 139

BTK

✿ Klassic / Konic	
Implant: Ø 3,25PL/3,75/4	
Platform: 4,1 ER (Code 0024)	p. 75
Implant: Ø 3,25/4	
Platform: 3,5 IR (Code 0040)	p. 87

B&W

✿ External Hexagon	
Implant: Ø 3,75/4	
Platform: 4,1 (Code 0024)	p. 75
Implant: Ø 5	
Platform: 5 (Code 0058)	p. 102

✿ Internal Hexagon	
Implant: Ø 3,3/4	
Platform: 4 (Code 0040)	p. 87

CAMLOG

★ Camlog Screw-Line	
Implant: Ø 3,8	
Platform: 3,8 (Code 0011)	p. 62
Implant: Ø 4,3	
Platform: 4,3 (Code 0012)	p. 63
★ Conelog Screw-Line	
Implant: Ø 3,8	
Platform: 3,8 (Code 0120)	p. 125
Implant: Ø 4,3	
Platform: 4,3 (Code 0121)	p. 126

CONEXÃO SISTEMA DE PRÓTESE

★ Flash	
Implant: Ø 3,5/4,3/5	
Platform: Universal (Code 0021)	p. 72
★ Torq	
Implant: Ø 3,5/3,75/4	
Platform: Universal (Code 0021)	p. 72
★ Expand	
Implant: Ø 3,75/4/5	
Platform: Universal (Code 0021)	p. 72

CORTEX

★ Dynamix	
Implant: Ø 3,3/3,8/4,2/5/6	
Platform: 3,75 (Code 0040)	p. 87
★ Classix	
Implant: Ø 3,3/3,8/4,2/5/6	
Platform: 3,75 (Code 0040)	p. 87
★ Saturn	
Implant: Ø 3,8/4,2	
Platform: 3,5 (Code 0040)	p. 87

★ Conical Platform:	
Implant: Ø 3	
Platform: NP (Code 0109)	p. 122
Implant: Ø 3,3/3,8/4,2	
Platform: RP (Code 0004)	p. 55
Implant: Ø 5/6	
Platform: WP (Code 0005)	p. 56
★ Magix	
Implant: Ø 3,3/3,8/4,2	
Platform: RP (Code 0004)	p. 55
★ Multi Unit	
Platform Universal (Code 0025)	p. 76

DENTAL TECH

★ Implogic	
Implant: Ø 4,5	
Platform: 4,5 (Blue) (Code 0041)	p. 89

DENTAURUM

★ Tiologic	
Implant: Ø 3,3	
Platform: Small (Code 0130)	p. 131
Implant: Ø 3,7/4,2	
Platform: Medium (Code 0131)	p. 132
Implant: Ø 4,8/5,5	
Platform: Large (Code 0132)	p. 133

DENTIS

★ s-Clean	
Implant: Ø 3,7	
Platform: Mini (Code 0030)	p. 81
Implant: Ø 4,1/4,3	
Platform: Regular (Code 0030)	p. 81
Implant: Ø 4,8	
Platform: Wide (Code 0030)	p. 81

DENTIUM

★ SimpleLine II	
Implant: Ø 3,8/4,3	
Platform: 4,8 (Code 0074)	p. 107
Implant: Ø 3,8/4,3	
Platform: 4,8 (Code 0037)	p. 84
Implant: Ø 4,3/4,8	
Platform: 6,5 (Code 0096)	p. 119
★ SuperLine and Implantium	
Implant: Ø 3,4	
Platform: 3,6 (Code 0030)	p. 81
Implant: Ø 3,8	
Platform: 4 (Code 0030)	p. 81
Implant: Ø 4,3	
Platform: 4,5 (Code 0030)	p. 81
Implant: Ø 4,8	
Platform: 5 (Code 0030)	p. 81
Implant: Ø 4,8	
Platform: 6 (Code 0030)	p. 81

★ Multi Unit SuperLine and Implantium	
Platform: 4,5 (Code 0193)	p. 161

★ NR Line	
Implant: Ø 3,1	
Platform: 3,2 (Code 0190)	p. 158
Implant: Ø 3,1	
Platform: 3,6 (Code 0190)	p. 158
Implant: Ø 3,6	
Platform: 3,6 (Code 0191)	p. 159
Implant: Ø 4,3	
Platform: 4,3 (Code 0191)	p. 159
Implant: Ø 5	
Platform: 5 (Code 0191)	p. 159
Implant: Ø 6	
Platform: 6 (Code 0191)	p. 159

★ Multi Unit NR Line	
Platform: 5 (Code 0192)	p. 160

DIO IMPLANTS

★ SM System	
Implant: Ø 4,5/5/5,3	
Platform: Regular/Wide (Code 0013)	p. 64
★ UF II Narrow	
Implant: Ø 3/3,3	
Platform: Narrow (Code 0014)	p. 65
★ UF II	
Implant: Ø 3,8/4/4,5/5/5,5	
Platform: Regular (Code 0030)	p. 81
★ External	
Implant: Ø 3,3/3,8	
Platform: Narrow 3,5 (Code 0023)	p. 74
Implant: Ø 3,75/4/4,5	
Platform: Regular 4,1 (Code 0024)	p. 75
Implant: Ø 5/5,3/5,5/6	
Platform: Wide 5,1 (Code 0061)	p. 105

EASY IMPLANT

★ Master C	
Implant: Ø 3,5	
Platform: 3,5 (Ocean) (Code 0004)	p. 55
Implant: Ø 4	
Platform: 4 (Ocean) (Code 0004)	p. 55
Implant: Ø 4,5	
Platform: 4,5 (Lilas) (Code 0030)	p. 81
Implant: Ø 5	
Platform: 5 (Lilas) (Code 0030)	p. 81
★ Master S	
Implant: Ø 3,3	
Platform: 3,3 (Ocean) (Code 0004)	p. 55
Implant: Ø 3,75	
Platform: 3,75 (Lilas) (Code 0030)	p. 81
Implant: Ø 4,25	
Platform: 4,25 (Lilas) (Code 0030)	p. 81
Implant: Ø 4,75	
Platform: 4,75 (Lilas) (Code 0030)	p. 81

★ Master L	
Implant: Ø 3,3	
Platform: 3,3 (Lilas) (Code 0030)	p. 81
Implant: Ø 3,75	
Platform: 3,75 (Lilas) (Code 0030)	p. 81
Implant: Ø 4,25	
Platform: 4,25 (Lilas) (Code 0030)	p. 81
Implant: Ø 4,75	
Platform: 4,75 (Lilas) (Code 0030)	p. 81
★ Multi Unit Conical Abutment	
Platform Universal (Code 0025)	p. 76

ECKERMANN

★ Hexagon	
Implant: Ø 3/3,5/4/4,5/5	
Platform: 4,1 (Code 0024)	p. 75

ELITE MEDICA

★ External Connection	
Implant: Ø 3,75	
Platform: Narrow (Code 0023)	p. 74
Implant: Ø 4	
Platform: Regular (Code 0024)	p. 75
Implant: Ø 5	
Platform: Wide (Code 0061)	p. 107

EUROTEKNIKA

★ Naturactis	
Implant: Ø 3,5	
Platform: 3,4 (Code 0004)	p. 55
Implant: Ø 4	
Platform: 3,8 (Code 0004)	p. 55
Implant: Ø 4,5	
Platform: 4,3 (Code 0004)	p. 55
Implant: Ø 5	
Platform: 4,8 (Code 0004)	p. 55

★ Uneva	
Implant: Ø 3,6	
Platform: 4,1 (Code 0024)	p. 75
Implant: Ø 4,1	
Platform: 4,1 (Code 0024)	p. 75
★ Uneva (Platform: Switching)	
Implant: Ø 4,8	
Platform: 4,1 (Code 0024)	p. 75
Implant: Ø 6	
Platform: 4,1 (Code 0024)	p. 75

★ Natea	
Implant: Ø 3,6/4,1/4,8	
Platform: Narrow (Code 0004)	p. 55
Implant: Ø 3,6/4,1/4,8	
Platform: Regular (Code 0004)	p. 55
Implant: Ø 6	
Platform: Wide (Code 0004)	p. 55

★ Aesthetica	
Implant: Ø 4,1	
Platform: 4,8 (Code 0074)	p. 107
Implant: Ø 4,1	
Platform: 4,8 (Code 0037)	p. 84
Implant: Ø 4,8	
Platform: 6,5 (Code 0096)	p. 119

★ Naturall	
Implant: Ø 3,5	
Platform: Narrow (Code 0004)	p. 55
Implant: Ø 4/4,5	
Platform: Regular (Code 0004)	p. 55
Implant: Ø 5	
Platform: Wide (Code 0004)	p. 55

★ Multi Unit Tetra	
Platform Universal (Code 0025)	p. 76

GALIMPLANT

✿ Internal Connection	
Implant: Ø 3,5	
Platform: 3,5 (Code 0004)	p. 55
Implant: Ø 4	
Platform: 4 (Code 0004)	p. 55
Implant: Ø 5	
Platform: 5 (Code 0004)	p. 55
✿ AbutmentMulti-Position	
Platform: Universal (Code 0025)	p. 76

GC TECH

✿ AADVA Standard / Tapered Implants	
Implant: Ø 3,3	
Platform: Narrow (Code 0196)	p. 162
Implant: Ø 4	
Platform: Regular (Code 0197)	p. 163
Implant: Ø 5	
Platform: Wide (Code 0198)	p. 164

GLOBAL D (TEKKA)

✿ In-Kone Universal	
Implant: Ø 3,5/4/4,5/5	
Platform: 5 (Code 0152)	p. 140
✿ In-Kone Primo	
Implant: Ø 3,5/4/4,5/5	
Platform: 5 (Code 0152)	p. 140

GMI (ILERIMPLANT)

✿ Phoenix	
Implant: Ø 3,3/3,75/4	
Platform: Standard 4,1 (Code 0024)	p. 75
Implant: Ø 5	
Platform: Wide 5,1 (Code 0061)	p. 105
✿ Frontier	
Implant: Ø 3,3/3,75/4,25	
Platform: RP 3,3 (Code 0040b)	p. 88
Implant: Ø 4,75/5,75	
Platform: WP 4,3 (Code 0041b)	p. 90
✿ Universal	
Platform: PS-RP 4,8 (Code 0025)	p. 76

GT MEDICAL

✿ Best Fit Internal Octagon	
Implant: Ø 3,7/4,3/4,8	
Platform: Regular (Code 0074)	p. 107
Implant: Ø 3,7/4,3/4,8	
Platform: Regular (Code 0037)	p. 84
✿ Best Fit Internal Hexagon	
Implant: Ø 3,7/4,1/4,3/4,8	
Platform: Wide (Code 0005)	p. 56
✿ Best Fit External Hexagon	
Implant: Ø 3,5	
Platform: Narrow (Code 0023)	p. 74
Implant: Ø 4,1	
Platform: Regular (Code 0024)	p. 75
Implant: Ø 5,1	
Platform: Wide (Code 0061)	p. 105

HAHN IMPLANT (GLIDEWELL)

✿ Hahn Tapered Implant	
Implant: Ø 3,5/4,3	
Platform: 3,5/4,3 (Code 0021)	p. 72
Implant: Ø 5	
Platform: 5 (Code 0022)	p. 73
Implant: Ø 7	
Platform: 7 (Code 0124)	p. 127
✿ Multi Unit Abutment system	
Platform: Universal (Code 0025)	p. 76

HI-TEC

✿ Tapered Self Thread	
Implant: Ø 3,3/3,75	
Platform: 3,5 (Code 0040)	p. 87
Implant: Ø 4,2/5	
Platform: 4,5 (Code 0041)	p. 89
✿ Logic Plus	
Implant: Ø 3,5	
Platform: 3,7 (Code 0040)	p. 87
Implant: Ø 4,3	
Platform: 3,9 (Code 0040)	p. 87

HIOSSEN

✿ ETTI SA/ETIII SA	
Implant: Ø 3,5	
Platform: Mini (Code 0029)	p. 80
Implant: Ø 4/4,5/5	
Platform: Regular (Code 0030)	p. 81
✿ ETTI BA	
Implant: Ø 3,5	
Platform: Mini (Code 0029)	p. 80
Implant: Ø 4/4,5/5	
Platform: Regular (Code 0030)	p. 81

IBS

✿ Magic FC	
Implant: Ø 4/4,5/5/5,5/6/6,5	
Platform: 3,8 (Code 0030)	p. 81
✿ N.R Fix	
Implant: Ø 3/3,5	
Platform: 3,8 (Code 0030)	p. 81

IDO IMPLANTS

✿ IDo Implant	
Implant: Ø 3,8/4/4,5/5/5,5/6/7	
Platform: Universal (Code 0030)	p. 81

IHDE DENTAL (IMBIODENT)

✿ Bone Level Plus	
Implant: Ø 3,3	
Platform: 3,3 (Code 0033)	p. 82
Implant: Ø 4,1	
Platform: 4,1 (Code 0035)	p. 83
Implant: Ø 4,8	
Platform: 4,8 (Code 0035)	p. 83

IMPLANT DIRECT

✿ RePlus / Replant / Reactive	
Implant: Ø 3,5/3,7/4,2	
Platform: 3,5 (Code 0026)	p. 77
Implant: Ø 4,3/4,7	
Platform: 4,3 (Code 0027)	p. 78
Implant: Ø 5/5,7	
Platform: 5 (Code 0028)	p. 79
✿ Legacy	
Implant: Ø 3,7/4,2	
Platform: 3,5 (Code 0040)	p. 87
Implant: Ø 4,7/5,2	
Platform: 4,5 (Code 0041)	p. 89

✿ Swishplant / Swishplus

Implant: Ø 4,1/4,8	
Platform: 4,8 (Code 0074)	p. 107
Implant: Ø 4,1/4,8	
Platform: 4,8 (Code 0037)	p. 84
Implant: Ø 4,8/5,7	
Platform: 6,5 (Code 0096)	p. 119

✿ SwishActive

Implant: Ø 3,3	
Platform: 3 (Code 0021)	p. 72
Implant: Ø 4,1/4,8	
Platform: 3,4 (Code 0022)	p. 73

✿ Interactive

Implant: Ø 3,2/3,7	
Platform: 3 (Code 0021)	p. 72
Implant: Ø 4,3/5	
Platform: 3,4 (Code 0022)	p. 73

IMPLANT GENESIS

✿ Aktiv System	
Implant: Ø 3,5/3,75/4,2/5	
Platform: Standard (Code 0040)	p. 87

INTRA-LOCK

✿ Unihex	
Implant: Ø 4	
Platform: Regular (Code 0024)	p. 75
✿ IntraHex	
Implant: Ø 3,75/4	
Platform: 3,5 (Code 0040)	p. 87
Implant: Ø 4,75	
Platform: 4,5 (Code 0041)	p. 89

JDENTALCARE

✿ JDEvolution/JDEvolution Plus	
Implant: Ø 3,7	
Platform: 3,7 (Code 0040)	p. 87
Implant: Ø 4,3/5	
Platform: 4 (Code 0040)	p. 87
Implant: Ø 6	
Platform: 5 (Code 0040)	p. 87
✿ JD ICON	
Implant: Ø 3,9	
Platform: 3,9 (Code 0022)	p. 73
Implant: Ø 4,3	
Platform: 4 (Code 0022)	p. 73
Implant: Ø 5	
Platform: 4,7 (Code 0022)	p. 73

KEYSTONE

✿ Internal TiLobe PrimaConnex	
Implant: Ø 3,3/3,5	
Platform: 3,5 (Code 0044)	p. 91
Implant: Ø 4/4,1	
Platform: 4,1 (Code 0045)	p. 92
Implant: Ø 5	
Platform: 5 (Code 0046)	p. 93
✿ Restore	
Implant: Ø 3,75/4	
Platform: RD 4,1 (Code 0024)	p. 75

KLOCKNER

✿ Essential Cone	
Implant: Ø 3,5/4/4,5	
Platform: 4,5 (Code 0054)	p. 100
✿ KL	
Implant: Ø 3,5	
Platform: Narrow (Code 0023)	p. 74
Implant: Ø 4,1	
Platform: Regular (Code 0024)	p. 75
Implant: Ø 5,1	
Platform: Wide (Code 0061)	p. 105
✿ Vega	
Implant: Ø 3,5	
Platform: NV (Code 0082)	p. 111
Implant: Ø 4/4,5	
Platform: RV (Code 0083)	p. 112

LASAK

✿ Bioniq	
Implant: Ø 2,9	
Platform: QN (Yellow) (Code 0166)	p. 148
Implant: Ø 3,5/4/5	
Platform: QR (Blue) (Code 0167)	p. 149
✿ Multi Unit	
Implant: Ø	
Platform: Universal (Code 0168)	p. 150

LEADER

✿ Tixos Internal Hex	
Implant: Ø 3,3	
Platform: 3,5 (Code 0040)	p. 87
Implant: Ø 3,75	
Platform: 4 (Code 0040)	p. 87
✿ Tixos External Hex	
Implant: Ø 3,3/3,75	
Platform: 4,1 (Code 0024)	p. 75
Implant: Ø 5	
Platform: 5 (Code 0058)	p. 102

MEDENTIS

✿ ICX-Templant	
Implant: Ø 3,75	
Platform: 3,75 (Code 0125)	p. 128
Implant: Ø 4,1	
Platform: 4,1 (Code 0125)	p. 128
Implant: Ø 4,8	
Platform: 4,8 (Code 0125)	p. 128

MEGAGEN

✿ AnyRidge	
Implant: Ø 3,5	
Platform: Small (Code 0015)	p. 66
Implant: Ø 4/4,5	
Platform: Regular (Code 0015)	p. 66
Implant: Ø 5/5,5	
Platform: Wide (Code 0015)	p. 66

✿ AnyOne Internal	
Implant: Ø 3,5/4/4,5/5/6/7	
Platform: General (Code 0030)	p. 81
✿ AnyOne External	
Implant: Ø 3,5	
Platform: Small 3,5 (Code 0023)	p. 74
Implant: Ø 4	
Platform: Regular 4,1 (Code 0024)	p. 75
Implant: Ø 4,5	
Platform: Regular 4,5 (Code 0024)	p. 75
Implant: Ø 5	
Platform: Wide 5 (Code 0058)	p. 102
Implant: Ø 6	
Platform: SuperWide 5,5 (Code 0058)	p. 102
✿ Cone Abutment	
Implant: Ø Universal	
Platform: 3,8 (Code 0128)	p. 129
Implant: Ø Universal	
Platform: 4,8 (Code 0074)	p. 107

✿ Mini Narrow Ridge	
Implant: Ø 3/3,4	
Platform: Mini (Code 0014)	p. 65
✿ Multi Unit N Type	
Platform: Universal (Code 0025)	p. 76

MICRODENT

✿ Universal	
Implant: Ø 3,3/3,5/3,75/4	
Platform: 4,1 (Code 0024)	p. 75
Implant: Ø 4,2/5	
Platform: 5,1 (Code 0058)	p. 102
✿ Ektos	
Implant: Ø 3,7/4,2	
Platform: 3,5 (Code 0040b)	p. 88

MIS

✿ Lance	
Implant: Ø 3,75/4,2	
Platform: Standard (Code 0024)	p. 75
Implant: Ø 5	
Platform: Wide (Code 0058)	p. 102
✿ Multi Unit	
Platform: General (Code 0020)	p. 71
✿ Seven	
Implant: Ø 3,3	
Platform: Narrow (Code 0019)	p. 70
Implant: Ø 3,75/4,2	
Platform: Standard (Code 0040)	p. 87
Implant: Ø 5/6	
Platform: Wide (Code 0041)	p. 89

✿ M4	
Implant: Ø 3,3	
Platform: Narrow (Code 0019)	p. 70
Implant: Ø 3,75/4,2	
Platform: Standard (Code 0040)	p. 87
Implant: Ø 5/6	
Platform: Wide (Code 0041)	p. 89

✿ C1	
Implant: Ø 3,3	
Platform: Narrow (Code 0016)	p. 67
Implant: Ø 3,75/4,2	
Platform: Standard (Code 0017)	p. 68
Implant: Ø 5	
Platform: Wide (Code 0018)	p. 69

✿ V3	
Implant: Ø 3,9/4,3/5	
Platform: Standard (Code 0017)	p. 68

MOZO-GRAU

✿ MG Osseous	
Implant: Ø 3,3	
Platform: 3,4 Mini (Code 0003)	p. 54
Implant: Ø 3,4/3,75/4,25	
Platform: 4,1 Standard (Code 0024)	p. 75
Implant: Ø 5	
Platform: 5 Maxi (Code 0061)	p. 105

✿ MG Inhex	
Implant: Ø 3,3	
Platform: 2,3 Mini (Code 0109)	p. 122
Implant: Ø 3,75/4,25	
Platform: 2,8 Standard (Code 0004)	p. 55
Implant: Ø 5	
Platform: 3,8 Maxi (Code 0005)	p. 56

MPI

✿ External Connection HE Privilege	
Implant: Ø 3,3	
Platform: 3,5 (Code 0009)	p. 60
Implant: Ø 3,3/4	
Platform: 4,1 (Code 0024)	p. 75
Implant: Ø 5	
Platform: 5 (Code 0058)	p. 102
✿ Privilege CM	
Implant: Ø 3,5/4	
Platform: Regular (Code 0004)	p. 55
Implant: Ø 5	
Platform: Wide (Code 0005)	p. 56
✿ Excellence CM	
Implant: Ø 3,5/4	
Platform: Regular (Code 0004)	p. 55
Implant: Ø 5	
Platform: Wide (Code 0005)	p. 56

NEOBIOTECH

✿ EB External System	
Implant: Ø 3,5	
Platform: Narrow (Code 0023)	p. 74
✿ IS Implant: System	
Implant: Ø 4	
Platform: Regular 4 (Code 0030)	p. 81
Implant: Ø 4,5	
Platform: Regular 4,5 (Code 0030)	p. 81
Implant: Ø 5	
Platform: Wide 5 (Code 0030)	p. 81
Platform: 4,8 (Code 0025)	p. 76

NEODENT

✿ Helix GM/Drive GM/Titamax GM	
Implant: Ø 3,5/3,75/4/4,3/5/6	
Platform: Regular (Code 0186)	p. 156
✿ Mini Pilar CM	
Platform: Universal (Code 0025)	p. 76

NEOSS

✿ ProActive Straight/Tapered	
Implant: Ø 3,5 Green	
Platform: ProActive (Code 0047)	p. 94
Implant: Ø 4 Yellow	
Platform: ProActive (Code 0047)	p. 94
Implant: Ø 4,5 Blue	
Platform: ProActive (Code 0048)	p. 95
Implant: Ø 5 Peach	
Platform: ProActive (Code 0048)	p. 95
Implant: Ø 5,5 Lilac	
Platform: ProActive (Code 0048)	p. 95

NOBEL BIOCARE

✿ Branemark	
Implant: Ø 3,3	
Platform: Narrow (Code 0023)	p. 74
Implant: Ø 3,75/4	
Platform: Regular (Code 0024)	p. 75
Implant: Ø 5/6	
Platform: Wide (Code 0061)	p. 105
✿ Multi Unit	
Platform: Regular (Code 0025)	p. 76

✿ Replace	
Implant: Ø 3,5 Platform: Narrow (Code 0026)	p. 77
Implant: Ø 4,3 Platform: Regular (Code 0027)	p. 78
Implant: Ø 5 Platform: Wide (Code 0028)	p. 79
Implant: Ø 6 Platform: Platform: 6 (Code 0129)	p. 130
✿ Active	
Implant: Ø 3 Platform: Mini 3.0 (Code 0159)	p. 141
Implant: Ø 3,5 Platform: Narrow (Code 0021)	p. 72
Implant: Ø 4,3/5 Platform: Regular (Code 0022)	p. 73
Implant: Ø 5,5 Platform: Wide (Code 0124)	p. 127
NORIS MEDICAL	
✿ Tuff	
Implant: Ø 3,3/3,75/4,2/5/6 Platform: 3,75 (Code 0040)	p. 87
✿ TuffTT	
Implant: Ø 3,3/3,75/4,2/5/6 Platform: 3,75 (Code 0040)	p. 87
✿ Onix	
Implant: Ø 3,3/3,75/4,2/5/6 Platform: 3,75 (Code 0040)	p. 87
✿ Cortical	
Implant: Ø 4,0/5/6 Platform: 3,75 (Code 0040)	p. 87

✿ PteryCore	
Implant: Ø 4,2 Platform: 3,75 (Code 0040)	p. 87
✿ PteryFit	
Implant: Ø 4,2 Platform: 3,75 (Code 0040)	p. 87
NORMON	
✿ Normoimplant HE	
Implant: Ø 3,25/3,75/4,25/4,75 Platform: 4,1 (Code 0024)	p. 75
✿ Normoimplant HI	
Implant: Ø 3,75/4,25/4,75 Platform: 3,5 (Code 0040b)	p. 88
NOVA IMPLANTS	
✿ PSI/PCI	
Implant: Ø 3,3/3,75/4,2/5/6 Platform: 3,75 (Code 0040b)	p. 88
OSSTEM IMPLANT	
✿ TS	
Implant: Ø 3,5 Platform: Mini (Code 0029)	p. 80
Implant: Ø 4/4,5/5/6/7 Platform: Regular (Code 0030)	p. 81
✿ US	
Implant: Ø 3,3/3,5 Platform: Mini 3,5 (Code 0023)	p. 74
Implant: Ø 3,75/4/4,5 Platform: Regular 4,1 (Code 0024)	p. 75
Implant: Ø 5/5,5 Platform: Wide 5,1 (Code 0061)	p. 105
Implant: Ø 5/5,5 Platform: Wide PS 5 (Code 0058)	p. 102

OSTEOPLUS	
✿ Shi	
Implant: Ø 3,3 / 3,75 / 4,2 Platform: 3,5 (Code 0040)	p. 87
PALTOP	
✿ Advanced classic	
Implant: Ø 3,75/4,2/5 Platform: Standard (Code 0040b)	p. 88
✿ Advanced +	
Implant: Ø 3,75/4,2/5 Platform: Standard (Code 0040b)	p. 88
✿ Dynamic	
Implant: Ø 3,75/4,2/5 Platform: Standard (Code 0040b)	p. 88
✿ DIVA	
Implant: Ø 3,75/4,2/5 Platform: Standard (Code 0040b)	p. 88
✿ Conical Active	
Implant: Ø 3,75/4,2/5 Platform: Standard (Code 0029)	p. 80
✿ Universal Multi Unit	
Platform: Universal (Code 0181)	p. 155
PHIBO	
✿ TSH/BNT Serie 3	
Implant: Ø 3,6 Platform: 4 (Code 0024)	p. 75
✿ TSH/BNT Serie 4	
Implant: Ø 4,2 Platform: 4 (Code 0024)	p. 75

PROCLINIC	
✿ Aqua CM	
Implant: Ø 3,5/4/5 Platform: 2,82 (Code 0004)	p. 55
✿ Cylindrical External/Conical External	
Implant: Ø 3,75/4,25//3,5/4 Platform: 4,1 Estandar (Code 0024)	p. 75
Implant: Ø 5 Platform: 5 Maxi (Code 0058)	p. 102
✿ Cylindrical Internal/Conical Internal	
Implant: Ø 3,3/3,75/4,25/5//3,5/4/5 Platform: 3,5 (Code 0040)	p. 87
✿ SP Octa	
Implant: Ø 3,3/4,1/4,8 Platform: 4,8 (Code 0074)	p. 107
Implant: Ø 3,3/4,1/4,8 Platform: 4,8 (Code 0037)	p. 84
Implant: Ø 4,8 Platform: 6,5 (Code 0096)	p. 119
RADHEX	
✿ PHI	
Implant: Ø 3,75 Platform: 3,5 (Code 0040b)	p. 88
Implant: Ø 4,5/5 Platform: 4,5 (Code 0041b)	p. 90
SEWON MEDIX	
✿ IH2 SLA SYSTEM	
Implant: Ø 3,5 Platform: Mini (Code 0029)	p. 80
Implant: Ø 3,5/4/4,5/5 Platform: Regular (Code 0030)	p. 81

✿ IH2 RBM SYSTEM	
Implant: Ø 3,5 Platform: Mini (Code 0029)	p. 80
Implant: Ø 3,5/4/4,5/5 Platform: Regular (Code 0030)	p. 81
✿ IH SYSTEM	
Platform: Universal (Code 0025)	p. 76
SGS	
✿ P1	
Implant: Ø 3,2/3,75/4,2/5/6 Platform: 3,75 (Code 0040)	p. 87
✿ P7	
Implant: Ø 3,2/3,75/4,2/4,5/5/6 Platform: 3,75 (Code 0040)	p. 87
SIC INVENT	
✿ Hexagonal System SICace	
Implant: Ø 3,4/4 Platform: 3,3 (Code 0170)	p. 152
Implant: Ø 4,5/5 Platform: 4,2 (Code 0171)	p. 153
SIGNO VINCES	
✿ Compact	
Implant: Ø 4,5 Platform: CM3,8 (Code 0004)	p. 55
✿ Duocon	
Implant: Ø 3,8 Platform: CM3,8 (Code 0004)	p. 55
Implant: Ø 4,6/5,5 Platform: CM4,6 (Code 0005)	p. 56
✿ Infra	
Implant: Ø 3,3/3,8/4,6 Platform: CM (Code 0004)	p. 55

SOUTHERN IMPLANTS	
✿ Tri-Nex	
Implant: Ø 3,5 Platform: 3,5 (Code 0026)	p. 77
Implant: Ø 4,3 Platform: 4,3 (Code 0027)	p. 78
Implant: Ø 5 Platform: 5 (Code 0028)	p. 79
Implant: Ø 6 Platform: 6 (Code 0129)	p. 130
✿ IT Connection	
Implant: Ø 3,3/4/4,1/4,9/5 Platform: 4,8 (Code 0037)	p. 84
Implant: Ø 4,9/5/6 Platform: 6,5 (Code 0096)	p. 119
✿ External Hex	
Implant: Ø 3,25 Platform: 3,4 (Code 0003)	p. 54
Implant: Ø 3,75/4 Platform: 4,1 (Code 0024)	p. 75
✿ Deep Conical	
Implant: Ø 3 Platform: 2,45 (Code 0109)	p. 122
Implant: Ø 3,5/4 Platform: 2,95/3,1 (Code 0004)	p. 55
Implant: Ø 5 Platform: 4,1 (Code 0005)	p. 56
✿ Internal Hex	
Implant: Ø 3,75/4,2/5 Platform: Universal (Code 0040)	p. 87
✿ Compact Conical	
Platform: 4,8 (Code 0025)	p. 76

STRAUMANN

✿ Tissue Level	
Implant: Ø 3,3/4,1/4,8	
Platform: Regular 4,8 (Code 0037)	p. 84
Implant: Ø 4,8	
Platform: Wide 6,5 (Code 0096)	p. 119
✿ Tissue Level NNC	
Implant: Ø 3,3	
Platform: 3,5 (Code 0160)	p. 142
✿ Synocta	
Implant: Ø 4,8	
Platform: Regular 4,8 (Code 0074)	p. 107
Implant: Ø 6,5	
Platform: Wide 6,5 (Code 0137)	p. 136
✿ Bone Level	
Implant: Ø 3,3	
Platform: NC- 3,3 (Code 0033)	p. 82
Implant: Ø 4,1	
Platform: RC-4,1 (Code 0035)	p. 83
Implant: Ø 4,8	
Platform: RC-4,8 (Code 0035)	p. 83
✿ Bone Level Tapered SC	
Implant: Ø 2,9	
Platform: SC- 2,9 (Code 0135)	p. 134
✿ Screw-Retained	
Implant: Ø Universal	
Platform: NC/RC (Code 0101)	p. 120
✿ BLX	
Implant: Ø 3,5/3,75/4/4,5	
Platform: RB (Regular Base) (Code 0207)	p. 166
Implant: Ø 5/5,5/6,5	
Platform: WB (Wide Base) (Code 0208)	p. 167

SYBRON IMPLANT SOLUTIONS

✿ Endopore (Innova)	
Implant: Ø 4,1	
Platform: 4,1 (Code 0024)	p. 75
TITANIUM-FIX	
✿ b-fix	
Implant: Ø 3,5/4	
Platform: Regular (Code 0004)	p. 55
Implant: Ø 4,5/5	
Platform: Larga (Code 0005)	p. 56

TRE-OSS

✿ Simple	
Implant: Ø 3,3/3,75/5	
Platform: 3,75 Amarillo (Code 0040)	p. 87

TRI DENTAL IMPLANTS

✿ TRI-Vent	
Implant: Ø 3,75/4,1/4,7	
Platform: 3,5 (Code 0040)	p. 87

TRINON

✿ Q2	
Implant: Ø 3,5/3,75/4,5	
Platform: 4 (Code 0024)	p. 75
✿ QK	
Implant: Ø 4	
Platform: 4,8 (Code 0074)	p. 107
Implant: Ø 4	
Platform: 4,8 (Code 0037)	p. 84

UFIT

✿ Gt2	
Implant: Ø 3,5	
Platform: Mini (Code 0004)	p. 55
Implant: Ø 4/4,5	
Platform: Regular (Code 0005)	p. 56
Implant: Ø 5	
Platform: Wide (Code 0005)	p. 56
Implant: Ø 5,5/6/6,5/7	
Platform: Ultra-wide (Code 0005)	p. 56
✿ Nt2	
Implant: Ø 3,5	
Platform: Mini (Code 0004)	p. 55
Implant: Ø 4/4,5	
Platform: Regular (Code 0005)	p. 56
Implant: Ø 5	
Platform: Wide (Code 0005)	p. 56
Implant: Ø 5,5/6/6,5/7	
Platform: Ultra-wide (Code 0005)	p. 56

VULKAN IMPLANTS

✿ IN-Hex	
Implant: Ø 3,3/3,75/4,2/5	
Platform: 3,75 (Code 0040)	p. 87

XIVE

✿ Xive	
Implant: Ø 3	
Platform: 3 (Code 0084)	p. 113
Implant: Ø 3,4	
Platform: 3,4 (Code 0038)	p. 85
Implant: Ø 3,8	
Platform: 3,8 (Code 0039)	p. 86
Implant: Ø 4,5	
Platform: 4,5 (Code 0085)	p. 114
Implant: Ø 5,5	
Platform: 5,5 (Code 0086)	p. 115

YES IMPLANT

✿ S-SYSTEM	
Implant: Ø 3,3/3,5	
Platform: Narrow (Code 0030)	p. 81
Implant: Ø 4/4,5	
Platform: Regular (Code 0030)	p. 81
Implant: Ø 5/5,5	
Platform: Wide (Code 0030)	p. 81

ZIACOM (OSSEOLIFE)

✿ OEX	
Implant: Ø 3,75/4,25	
Platform: RP 4,1 (Code 0024)	p. 75

ZIMMER

✿ Eztetic	
Implant: Ø 3,1	
Platform: 2,9 (Code 0178)	p. 154
✿ Screw-Vent	
Implant: Ø 3,7/4,1	
Platform: 3,5 (Code 0040)	p. 87
Implant: Ø 4,7	
Platform: 4,5 (Code 0041)	p. 89
Implant: Ø 6	
Platform: 5,7 (Code 0080)	p. 109
✿ Swiss-Plus	
Implant: Ø 3,7/4,1/4,8	
Platform: 4,8 (Code 0074)	p. 107
Implant: Ø 3,7/4,1/4,8	
Platform: 4,8 (Code 0037)	p. 84
✿ Tapered Abutment Multi Unit	
Implant: Ø Universal	
Platform: Universal (Code 0205)	p. 165

COMPATIBLE with 0001

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c
0,3 mm				1,2 mm				mm				mm			
R	31.322.001.01-2	43°	25°	31.322.001.02-2	25°	-	-	-	-	-	-	-	-	-	-
NR	31.312.001.01-2			31.312.001.02-2			-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
0,3 mm		CH=5mm	CH= 7mm	CH= 9mm
R	31.322.001.21-2	25°	20°	10°
NR	31.312.001.21-2			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL			SCANALOG
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT- CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}	
52.410.103.01-2	10	50.312.001.01-2	43.621.410.01-2	34.612.001.01-2	32.212.001.02-2	25°	33.390.754.01-2	3	25°	23.412.001.01-2
			43.624.410.01-2				33.490.754.01-2	4		
52.412.103.01-2	12		43.630.410.01-2				33.690.754.01-2	6		

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.20				
41.316.084.01-2	-	43.618.201.01-2	18	40.316.003.01-2	43.601.103.02-2	22.612.001.01-2	30.412.001.01-2		
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES



STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0001	LAB SCANBODY	DAS_C_E_0001
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0001	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0001
	DAS_I_12_0001		DAS_C_I_12_0001
SCANALOG	DAS_SA_0001	SCANALOG	DAS_C_SA_0001

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0002

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c
0,3 mm				1,2 mm				mm				mm			
R	31.323.002.01-2	45°	20°	31.323.002.02-2	25°	-	-	-	-	-	-	-	-	-	-
NR	31.313.002.01-2			31.313.002.02-2		-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
0,3 mm		CH=5mm	CH= 7mm	CH= 9mm
R	31.323.002.21-2	25°	20°	10°
NR	31.313.002.21-2			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL			SCANALOG	
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT- CHROME		α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}	
52.408.101.01-2	8	50.313.002.01-2	43.621.410.01-2	34.613.002.01-2	32.213.002.02-2		30°	33.390.805.01-2	3	30°	23.413.002.01-2
52.410.101.01-2	10		43.624.410.01-2					33.490.805.01-2	4		
52.412.101.01-2	12		43.630.410.01-2					33.690.805.01-2	6		

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.20				
41.316.084.01-2	-	43.618.201.01-2	18	40.316.003.01-2	43.601.103.02-2	22.613.002.01-2	30.413.002.01-2		
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES



STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0002	LAB SCANBODY	DAS_C_E_0002
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_8_0002	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_8_0002
	DAS_I_10_0002		DAS_C_I_10_0002
	DAS_I_12_0002		DAS_C_I_12_0002
	DAS_I_12_0002		DAS_C_I_12_0002
SCANALOG	DAS_SA_0002	SCANALOG	DAS_C_SA_0002

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0003

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c
0,3 mm				0,5 mm				mm				mm			
R	31.322.003.01-2	45°	30°	31.322.003.02-2	25°	-	-	-	-	-	-	-	-	-	-
NR	31.312.003.01-2			31.312.003.01-2			-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
1 mm		CH=5mm	CH= 7mm	CH= 9mm
R	31.322.003.23-2	30°	25°	15°
NR	31.312.003.23-2			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}
52.410.104.01-2	10	50.312.003.01-2	43.621.410.01-2	34.612.003.01-2	-	-	33.390.716.01-2	3	25°
			43.624.410.01-2				33.490.716.01-2	4	
52.412.104.01-2	12		43.630.410.01-2				33.690.716.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.20				
41.320.065.01-2	-	43.618.201.01-2	18	40.320.003.02-2	43.601.103.02-2	22.612.003.01-2	30.412.001.01-2		
		43.624.201.01-2	24						
		43.632.201.01-2	32						


LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0003	LAB SCANBODY	DAS_C_E_0003
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0003	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0003
	DAS_I_12_0003		DAS_C_I_12_0003

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

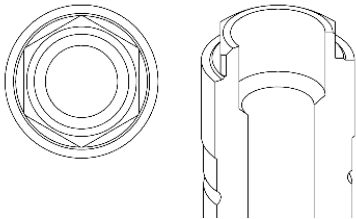

COMPATIBLE with 0004

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c
1 mm				2 mm				3 mm				4 mm			
R	31.323.004.01-2	45°	29°	31.323.004.02-2	30°	20°	-	31.323.004.03-2	25	-	-	31.323.004.04-2	20	-	-
NR	31.313.004.01-2			31.313.004.02-2				31.313.004.03-2				31.313.004.04-2			

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
1 mm		CH=5mm	CH= 7mm	CH= 9mm
R	31.323.004.21-2	25°	20°	10°
NR	31.313.004.21-2			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL			SCANALOG
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}	
52.410.103.01-2	10	50.313.004.01-2	43.620.411.01-2	34.613.004.01-2 (1) 34.613.004.02-2 (2)	32.213.004.02-2	25°	33.390.754.01-2	3	25°	23.413.004.01-2
			43.621.410.01-2				33.490.754.01-2	4		
52.412.103.01-2	12	50.313.004.03-2 (IG=3mm)	43.624.410.01-2				33.690.754.01-2	6		
			43.630.410.01-2							

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27				
41.316.076.01-2	-	43.618.201.01-2	18	40.316.005.02-2	43.601.105.01-2	22.613.004.01-2	30.413.002.01-2		
		43.624.201.01-2	24						
		43.632.201.01-2	32						


LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0004	LAB SCANBODY	DAS_C_E_0004
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0004 DAS_IG_10_0004	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0004 DAS_C_IG_10_0004
	DAS_I_12_0004 DAS_IG_12_0004		DAS_C_I_12_0004 DAS_C_IG_12_0004
SCANALOG	DAS_SA_0004	SCANALOG	DAS_C_SA_0004

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height
IG = Adaptor 3mm

α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

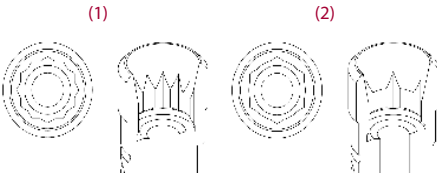

COMPATIBLE with 0005

STANDARD DYNAMIC TIBASE®													
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT	
1 mm				2 mm				3 mm				4 mm	
R	31.324.005.01-2	38°	23°	31.324.005.02-2	25°	15°	-	31.324.005.03-2	20	-	-	-	-
NR	31.314.005.01-2			31.314.005.02-2				31.314.005.03-2				-	

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
1 mm		CH=5mm	CH= 7mm	CH= 9mm
R	31.324.005.21-2	25°	20°	10°
NR	31.314.005.21-2			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME		DYNAMIC MILLING TOOL	SHANK	α _{di}
52.410.102.01-2	10	50.314.005.01-2	43.620.411.01-2	34.614.005.01-2	-	-	33.390.958.01-2	3	30°
			43.621.410.01-2				33.490.958.01-2	4	
52.412.102.01-2	12		43.624.410.01-2 (IG=3mm)				33.690.958.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27	LAB SCANBODY	
41.320.090.01-2	-	43.618.201.01-2	18	40.320.005.03-2	43.601.105.01-2	22.614.005.01-2	30.413.002.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				



LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0005	LAB SCANBODY	DAS_C_E_0005
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0005	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0005
	DAS_IG_10_0005		DAS_C_IG_10_0005
	DAS_I_12_0005		DAS_C_I_12_0005
	DAS_IG_12_0005		DAS_C_IG_12_0005

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height
IG = Adaptor (3mm)

α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0006

STANDARD DYNAMIC TIBASE®													
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT	
1,2 mm				2 mm				3 mm				4 mm	
R	31.322.006.01-2	40°	20°	31.322.006.02-2	25	-	-	31.322.006.03-2	20	-	-	31.322.006.04-2	15
NR	31.312.006.01-2			31.312.006.02-2				31.312.006.03-2				31.312.006.04-2	

DYNAMIC 3TIBASE®			
GINGIVAL HEIGHT		α _s	α _s
		CH=5mm	CH= 7mm
R	-	-	-
NR	-		

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL			SCANALOG
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME		DYNAMIC MILLING TOOL	SHANK	α _{di}	
52.410.105.01-2	10	50.312.006.01-2	43.621.410.01-2	34.612.006.01-2	32.212.006.02-2	25°	33.330.734.01-2	3	25°	23.412.006.01-2
			43.624.410.01-2				33.430.734.01-2	4		
52.412.105.01-2	12		43.630.410.01-2				33.630.734.01-2	6		

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27	LAB SCANBODY	
41.316.072.01-2	-	43.618.201.01-2	18	40.316.005.01-2	43.601.105.01-2	22.612.006.01-2	30.412.001.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				



LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0006	LAB SCANBODY	DAS_C_E_0006
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0006	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0006
	DAS_I_12_0006		DAS_C_I_12_0006
SCANALOG	DAS_SA_0006	SCANALOG	DAS_C_SA_0006

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0007

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c
1,5 mm				mm			mm			mm			mm		
R	31.323.007.01-2	38°	17°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.007.01-2			-			-			-			-		

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
1,5 mm		CH=5mm	CH= 7mm	CH= 9mm
R	31.323.007.21-2	25°	20°	10°
NR	31.313.007.21-2			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}
52.408.101.01-2	8	50.313.007.01-2	43.621.410.01-2	34.613.007.01-2	32.213.007.02-2	25°	33.350.775.01-2	3	25°
52.410.101.01-2	10		43.624.410.01-2				33.450.775.01-2	4	
52.412.101.01-2	12		43.630.410.01-2				33.650.775.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27				
41.318.074.01-2	-	43.618.201.01-2	18	40.318.005.02-2	43.601.105.01-2	22.613.007.01-2	30.413.002.01-2		
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES



STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0007	LAB SCANBODY	DAS_C_E_0007
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_8_0007	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_8_0007
	DAS_I_10_0007		DAS_C_I_10_0007
	DAS_I_12_0007		DAS_C_I_12_0007

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0008

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c
0,5 mm				mm			mm			mm			mm		
R	31.323.008.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	-			-			-			-			-		

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
0,5 mm		CH=5mm	CH= 7mm	CH= 9mm
R	31.323.008.21-2	25°	20°	10°
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL			SCANALOG
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}	
52.408.113.01-2	8	50.313.008.01-2	43.621.410.01-2	34.613.008.01-2	-	-	33.370.716.01-2	3	30°	23.413.008.01-2
			43.624.410.01-2				33.470.716.01-2	4		
			43.630.410.01-2				33.670.716.01-2	6		

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27				
41.318.045.01-2	-	43.618.201.01-2	18	40.318.005.01-2	43.601.105.01-2			-	30.412.001.01-2
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES



STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0008	LAB SCANBODY	DAS_C_E_0008
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_8_0008	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_8_0008
SCANALOG	DAS_SA_0008	SCANALOG	DAS_C_SA_0008

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0009

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c
0,3 mm				0,5 mm				1 mm				mm			
R	31.322.009.01-2	45°	25°	31.322.009.02-2	25°	25°	31.322.009.03-2	25°	-	-	-	-	-	-	-
NR	31.312.009.01-2			31.312.009.02-2			31.312.009.03-2			-					

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME		DYNAMIC MILLING TOOL	SHANK	α _{di}
52.410.114.01-2	10	50.312.009.01-2	43.621.410.01-2	34.612.009.01-2	-	-	33.390.716.01-2	3	25°
			43.624.410.01-2				33.490.716.01-2	4	
52.412.114.01-2	12		43.630.410.01-2				33.690.716.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.20	ANALOG	LAB SCANBODY
41.320.051.01-2	-	43.618.201.01-2	18	40.320.003.01-2	43.601.103.02-2	22.612.009.01-2	30.412.001.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES



STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0009	LAB SCANBODY	DAS_C_E_0009
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0009	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0009
	DAS_I_12_0009		DAS_C_I_12_0009

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0010

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c
0,3 mm				mm				mm				mm			
R	31.323.010.01-2	45°	29°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.010.01-2			-			-		-						

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME		DYNAMIC MILLING TOOL	SHANK	α _{di}
52.410.115.01-2	10	50.313.010.01-2	43.621.410.01-2	34.613.010.01-2	-	-	33.390.716.01-2	3	30°
			43.624.410.01-2				33.490.716.01-2	4	
52.412.115.01-2	12	50.313.010.04-2 (IG=3mm)	43.630.410.01-2				33.690.716.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.20	ANALOG	LAB SCANBODY
41.318.065.01-2	-	43.618.201.01-2	18	40.318.003.01-2	43.601.103.02-2	22.613.010.01-2	30.413.002.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES



STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0010	LAB SCANBODY	DAS_C_E_0010
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0010 DAS_IG_10_0010	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0010 DAS_C_IG_10_0010
	DAS_I_12_0010 DAS_IG_12_0010		DAS_C_I_12_0010 DAS_C_IG_12_0010

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height
IG = Adaptor 3mm

α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0011

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c
0,3 mm				mm			mm			mm			mm		
R	31.322.011.01-2	25°	29°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.312.011.01-2			-			-			-			-		

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}
52.410.108.01-2	10	50.312.011.01-2	43.621.410.01-2	34.612.011.01-2	-	-	33.345.804.01-2	3	20°
			43.624.410.01-2				33.445.804.01-2	4	
52.412.108.01-2	12		43.630.410.01-2				33.645.804.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27	ANALOG	LAB SCANBODY
41.316.094.01-2	-	43.618.201.01-2	18	40.316.005.04-2	43.601.105.01-2	-	30.412.001.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES



STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0011	LAB SCANBODY	DAS_C_E_0011
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0011	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0011
	DAS_I_12_0011		DAS_C_I_12_0011

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0012

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c
0,3 mm				mm			mm			mm			mm		
R	31.323.012.01-2	25°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.012.01-2			-			-			-			-		

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}
52.410.109.01-2	10	50.313.012.01-2	43.621.410.01-2	34.613.012.01-2	-	-	33.345.804.01-2	3	20°
			43.624.410.01-2				33.445.804.01-2	4	
52.412.109.01-2	12		43.630.410.01-2				33.645.804.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27	ANALOG	LAB SCANBODY
41.316.094.01-2	-	43.618.201.01-2	18	40.316.005.04-2	43.601.105.01-2	-	30.413.002.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES



STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0012	LAB SCANBODY	DAS_C_E_0012
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0012	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0012
	DAS_I_12_0012		DAS_C_I_12_0012

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0013

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c
0,7 mm				mm			mm			mm			mm		
R	31.323.013.01-2	43°	23°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.013.01-2			-			-			-			-		

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}
-	-	-	-	-		-	-	-	-	-
-	-							-	-	
-	-							-	-	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER TORX T6	ANALOG	LAB SCANBODY
41.320.074.01-2	-	43.618.201.01-2	18	40.320.007.02-2	43.601.107.01-2	-	30.413.002.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

COMPATIBLE with 0014

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c
1,2 mm				2 mm				3 mm				mm			
R	31.322.014.01-2	41°	23°	31.322.014.02-2	25°	17°	-	20°	25°	-	-	-	-	-	-
NR	31.312.014.01-2			31.312.014.02-2			31.312.014.03-2			-			-		

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL			SCANALOG
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}	
52.410.128.01-2	10	50.312.014.03-2 (IG=3mm)	43.621.415.01-2	-		-	-	33.345.804.01-2	3	25°	23.412.014.01-2
-	-							33.445.804.01-2	4		
-	-							33.645.804.01-2	6		

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.20	ANALOG	LAB SCANBODY
41.314.067.01-2	41.314.105.01-2	43.618.201.01-2	18	40.314.003.04-2	43.601.103.02-2	-	30.412.001.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

COMPATIBLE with 0015

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c
1,7 mm				2,5 mm				mm				mm			
R	31.323.015.01-2	43°	23°	31.323.015.02-2	25°	15°	-	-	-	-	-	-	-	-	-
NR	31.313.015.01-2			31.313.015.02-2			-					-			

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
1,7 mm		CH=5mm	CH= 7mm	CH= 9mm
R	31.323.015.21-2	30°	25°	10°
NR	31.313.015.21-2			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL			SCANALOG
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT- CHROME		α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}
52.410.104.01-2	10	50.313.015.01-2	43.621.410.01-2	34.613.015.01-2	-	-	33.390.805.01-2	3	25°	23.413.015.01-2
			43.624.410.01-2				33.490.805.01-2	4		
52.412.104.01-2	12	50.313.015.03-2 (IG=3mm)	43.630.410.01-2				33.690.805.01-2	6		



DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.20	ANALOG	LAB SCANBODY
41.318.080.01-2	-	43.618.201.01-2	18	40.318.003.02-2	43.601.103.02-2	-	30.413.002.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0015	LAB SCANBODY	DAS_C_E_0015
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0015 DAS_IG_10_0015	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0015 DAS_C_IG_10_0015
	DAS_I_12_0015 DAS_IG_12_0015		DAS_C_I_12_0015 DAS_C_IG_12_0015
	SCANALOG	SCANALOG	DAS_C_SA_0015

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height
IG = Adaptador (3mm)
α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0016

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c
0,8 mm				mm				mm				mm			
R	31.322.016.01-2	45°	28°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.312.016.01-2			-				-				-			

DYNAMIC 3TIBASE®			
GINGIVAL HEIGHT		α _s	α _s
		CH=5mm	CH= 7mm
R	-	-	-
NR	-		

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT- CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}
52.408.106.01-2	8	50.312.016.01-2	43.621.410.01-2	34.612.016.01-2	-	-	33.360.754.01-2	3	25°
52.410.106.01-2	10		43.624.410.01-2				33.460.754.01-2	4	
52.412.106.01-2	12		43.630.410.01-2				33.660.754.01-2	6	



DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27	ANALOG	LAB SCANBODY
41.316.071.01-2	-	43.618.201.01-2	18	40.316.005.05-2	43.601.105.01-2	-	30.412.001.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0016	LAB SCANBODY	DAS_C_E_0016
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_8_0016	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_8_0016
	DAS_I_10_0016		DAS_C_I_10_0016
	DAS_I_12_0016		DAS_C_I_12_0016

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height
α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0017

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c
0,7 mm				mm			mm			mm			mm		
R	31.323.017.01-2	45°	24°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.017.01-2			-			-			-			-		

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
0,7 mm		CH=5mm	CH= 7mm	CH= 9mm
R	31.323.017.21-2	30°	25°	15°
NR	31.313.017.21-2			

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}
52.408.101.01-2	8	50.313.017.01-2	43.621.410.01-2	34.613.017.01-2		-	-	33.360.756.01-2	3	30°
52.410.101.01-2	10		43.624.410.01-2					33.460.756.01-2	4	
52.412.101.01-2	12		43.630.410.01-2					33.660.756.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27	ANALOG	LAB SCANBODY
41.317.073.01-2	-	43.618.201.01-2	18	40.317.005.01-2	43.601.105.01-2	-	30.413.002.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				


LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0017	LAB SCANBODY	DAS_C_E_0017
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_8_0017	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_8_0017
	DAS_I_10_0017		DAS_C_I_10_0017
	DAS_I_12_0017		DAS_C_I_12_0017

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

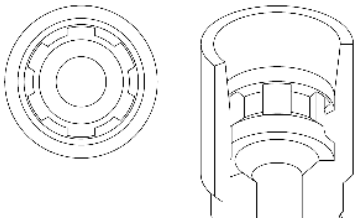

COMPATIBLE with 0018

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c
1,2 mm				mm			mm			mm			mm		
R	31.324.018.01-2	39°	18°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.314.018.01-2			-			-			-			-		

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}
52.410.102.01-2	10	50.314.018.01-2	43.621.410.01-2	34.614.018.01-2		-	-	33.360.756.01-2	3	30°
			43.624.410.01-2					33.460.756.01-2	4	
52.412.102.01-2	12		43.630.410.01-2					33.660.756.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27	ANALOG	LAB SCANBODY
41.317.073.01-2	-	43.618.201.01-2	18	40.317.005.01-2	43.601.105.01-2	-	30.413.002.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				


LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0018	LAB SCANBODY	DAS_C_E_0018
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0018	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0018
	DAS_I_12_0018		DAS_C_I_12_0018

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

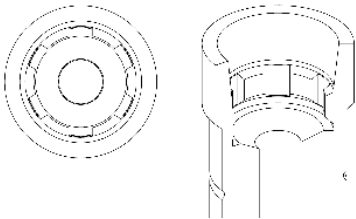

COMPATIBLE with 0019

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c
0,8 mm				mm			mm			mm			mm		
R	31.322.019.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.312.019.01-2			-			-			-			-		

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}
52.410.105.01-2	10	50.312.019.01-2	43.621.410.01-2	34.612.019.01-2	-	-	33.360.754.01-2	3	25°
			43.624.410.01-2				33.460.754.01-2	4	
52.412.105.01-2	12		43.630.410.01-2				33.660.754.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27	ANALOG	LAB SCANBODY
41.316.071.01-2	-	43.618.201.01-2	18	40.316.005.05-2	43.601.105.01-2	-	30.412.001.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES



STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0019	LAB SCANBODY	DAS_C_E_0019
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0019	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0019
	DAS_I_12_0019		DAS_C_I_12_0019

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0020

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c
0,6 mm				mm			mm			mm			mm		
R	31.323.020.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	-			-			-			-			-		

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}
52.408.112.01-2	8	50.313.020.01-2	43.620.411.01-2	34.613.020.01-2	-	-	33.390.716.01-2	3	30°
-	10						33.490.716.01-2	4	
-	12						33.690.716.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27	ANALOG	LAB SCANBODY
41.316.044.01-2	-	43.618.201.01-2	18	40.316.005.06-2	43.601.105.01-2	-	30.413.005.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0020	LAB SCANBODY	DAS_C_E_0020
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_8_0020	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_8_0020

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0021

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c
1,5 mm				2 mm				3 mm				4 mm			
R	31.322.021.01-2	43°	24°	31.322.021.02-2	25°	20°	31.322.021.03-2	20°	25°	31.322.021.04-2	15°	25°	-	-	-
NR	31.312.021.01-2			31.312.021.02-2			31.312.021.03-2			31.312.021.04-2			-		

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
1,5 mm		CH=5mm	CH= 7mm	CH= 9mm
R	31.322.021.21-2	25°	20°	10°
NR	31.312.021.21-2			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL			SCANALOG	
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT- CHROME		α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}	
52.410.103.01-2	10	50.312.021.01-2	43.621.410.01-2	34.612.021.01-2	32.212.021.02-2	25°	33.335.754.01-2	3	25°	23.412.021.01-2	
			43.624.410.01-2				33.435.754.01-2	4			
52.412.103.01-2	12	50.312.021.03-2 (IG=3mm)	43.630.410.01-2				33.635.754.01-2	6			


DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER UNIGRIP	ANALOG	LAB SCANBODY
41.316.073.01-2	-	43.618.201.01-2	18	40.316.008.02-2	43.601.108.01-2	22.612.021.01-2	30.412.001.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0021	LAB SCANBODY	DAS_C_E_0021
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0021	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0021
	DAS_IG_10_0021		DAS_C_IG_10_0021
	DAS_I_12_0021		DAS_C_I_12_0021
	DAS_IG_12_0021		DAS_C_IG_12_0021
SCANALOG	DAS_SA_0021	SCANALOG	DAS_C_SA_0021

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height
IG = Adaptor (3mm)
α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

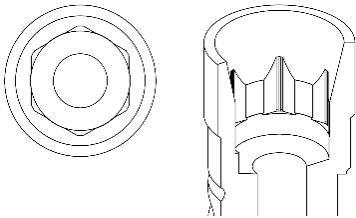

COMPATIBLE with 0022

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c
1,3 mm				2 mm				3 mm				4 mm			
R	31.323.022.01-2	40°	19°	31.323.022.02-2	25°	14°	31.323.022.03-2	20°	30°	-	15	30	-	-	-
NR	31.313.022.01-2			31.313.022.02-2			31.313.022.03-2			31.313.022.04-2			-		

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
1,3 mm		CH=5mm	CH= 7mm	CH= 9mm
R	31.323.022.21-2	30°	25°	10°
NR	31.313.022.21-2			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL			SCANALOG
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT- CHROME		α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}
52.408.101.01-2	8	50.313.022.01-2 50.313.022.03-2 (IG=3mm)	43.621.410.01-2	34.613.022.01-2	32.213.022.02-2	30°	33.335.758.01-2	3	30°	23.413.022.01-2
52.410.101.01-2	10		43.624.410.01-2				33.435.758.01-2	4		
52.412.101.01-2	12		43.630.410.01-2				33.635.758.01-2	6		


DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER UNIGRIP	ANALOG	LAB SCANBODY
41.320.075.01-2	-	43.618.201.01-2	18	40.320.008.02-2	43.601.108.01-2	22.613.022.01-2	30.413.002.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0022	LAB SCANBODY	DAS_C_E_0022
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_8_0022	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_8_0022
	DAS_IG_8_0022		DAS_C_IG_8_0022
	DAS_I_10_0022		DAS_C_I_10_0022
	DAS_IG_10_0022		DAS_C_IG_10_0022
	DAS_I_12_0022		DAS_C_I_12_0022
	DAS_IG_12_0022		DAS_C_IG_12_0022
SCANALOG	DAS_SA_0022	SCANALOG	DAS_C_SA_0022

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height
IG = Adaptor (3mm)
α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

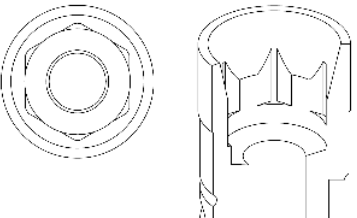

COMPATIBLE with 0023

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c
0,3 mm				mm				mm				mm			
R	31.322.023.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.312.023.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	α _s	α _s	α _s
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL			SCANALOG
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT- CHROME		α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}
52.410.103.01-2	10	50.312.023.01-2	43.621.410.01-2	34.612.023.01-2	-	-	33.390.805.01-2	3	25°	23.412.023.01-2
			43.624.410.01-2				33.490.805.01-2	4		
52.412.103.01-2	12		43.630.410.01-2				33.690.805.01-2	6		

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER UNIGRIP	ANALOG	LAB SCANBODY
41.316.059.01-2	-	43.618.201.01-2	18	40.316.008.01-2	43.601.108.01-2	22.612.023.01-2	30.412.001.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES



STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0023	LAB SCANBODY	DAS_C_E_0023
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0023	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0023
	DAS_I_12_0023		DAS_C_I_12_0023
SCANALOG	DAS_SA_0023	SCANALOG	DAS_C_SA_0023

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0024

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c
	0,3 mm			0,5 mm			mm			mm			mm		
R	31.323.024.01-2	45°	30°	31.323.024.02-2	30°	30°	-	-	-	-	-	-	-	-	-
NR	31.313.024.01-2			31.313.024.02-2			-			-			-		

DYNAMIC 3TIBASE®																	
		GINGIVAL HEIGHT	α _s	α _s	α _s	GINGIVAL HEIGHT	α _s	α _s	α _s	GINGIVAL HEIGHT	α _s	α _s	α _s	GINGIVAL HEIGHT	α _s	α _s	α _s
		0,3 mm	CH 5mm	CH 7mm	CH 9mm	0,5 mm	CH 5mm	CH 7mm	CH 9mm	1 mm	CH 5mm	CH 7mm	CH 9mm	2 mm	CH 5mm	CH 7mm	CH 9mm
R	31.323.024.21-2	30°	25°	10°	31.323.024.22-2	30°	25°	10°	31.323.024.23-2	30°	25°	10°	31.323.024.24-2	30°	25°	10°	
NR	31.313.024.21-2				31.313.024.22-2				31.313.024.23-2				31.313.024.24-2				

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL			SCANALOG
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT- CHROME		α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}
52.408.101.01-2	8	50.313.024.01-2	43.621.410.01-2	34.613.024.01-2	-	-	33.390.716.01-2	3	30°	23.413.024.01-2
52.410.101.01-2	10		43.624.410.01-2				33.490.716.01-2	4		
52.412.101.01-2	12		43.630.410.01-2				33.690.716.01-2	6		

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER UNIGRIP	ANALOG	LAB SCANBODY
41.320.060.01-2	-	43.618.201.01-2	18	40.320.008.01-2	43.601.108.01-2	22.613.024.01-2	30.413.002.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES



STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0024	LAB SCANBODY	DAS_C_E_0024
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_8_0024	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_8_0024
	DAS_I_10_0024		DAS_C_I_10_0024
	DAS_I_12_0024		DAS_C_I_12_0024
SCANALOG	DAS_SA_0024	SCANALOG	DAS_C_SA_0024

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0025

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c
0,3 mm				mm				mm				mm			
R	31.323.025.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	-			-			-		-						

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
0,3 mm		CH=5mm	CH= 7mm	CH= 9mm
R	31.323.025.21-2	30°	25°	10°
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL			SCANALOG
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT- CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}	
52.408.112.01-2	8	50.313.025.02-2	43.620.411.01-2	34.613.025.01-2	-	-	33.390.716.01-2	3	30°	23.413.025.01-2
52.410.111.01-2	10	50.313.025.01-2	43.621.410.01-2 43.624.410.01-2 43.630.410.01-2				33.490.716.01-2	4		
							33.690.716.01-2	6		

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER UNIGRIP	LAB SCANBODY	
41.314.039.01-2	-	43.618.201.01-2	18	40.314.008.01-2	43.601.108.01-2	22.613.025.01-2 30.413.005.01-2	
		43.624.201.01-2	24				
		43.632.201.01-2	32				

COMPATIBLE with 0026

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c
0,5 mm				1,2 mm				mm				mm			
R	31.322.026.01-2	45°	29°	31.322.026.02-2	25°	22°	-	-	-	-	-	-	-	-	-
NR	31.312.026.01-2			31.312.026.02-2			-			-					

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
0,5 mm		CH=5mm	CH= 7mm	CH= 9mm
R	31.322.026.21-2	25°	20°	10°
NR	31.312.026.21-2			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT- CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}
52.410.108.01-2	10	50.312.026.01-2	43.621.410.01-2	34.612.026.01-2	-	-	33.390.805.01-2	3	25°
			43.624.410.01-2				33.490.805.01-2	4	
52.412.108.01-2	12		43.630.410.01-2				33.690.805.01-2	6	


DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER UNIGRIP	LAB SCANBODY	
41.318.075.01-2	-	43.618.201.01-2	18	40.318.008.01-2	43.601.108.01-2	22.612.026.01-2 30.412.001.01-2	
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES			
STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0026	LAB SCANBODY	DAS_C_E_0026
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0026	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0026
	DAS_I_12_0026		DAS_C_I_12_0026

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

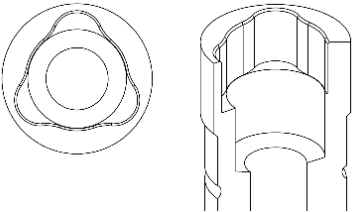

COMPATIBLE with 0027

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c
0,3 mm				1,2 mm				mm				mm			
R	31.323.027.01-2	35°	29°	31.323.027.02-2	25°	22°	-	-	-	-	-	-	-	-	-
NR	31.313.027.01-2			31.313.027.02-2			-					-			

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
0,3 mm		CH=5mm	CH= 7mm	CH= 9mm
R	31.323.027.21-2	25°	20°	10°
NR	31.313.027.21-2			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}
52.410.109.01-2	10	50.313.027.01-2	43.621.410.01-2	34.613.027.01-2	-	-	33.390.958.01-2	3	30°
			43.624.410.01-2				33.490.958.01-2	4	
52.412.109.01-2	12		43.630.410.01-2				33.690.958.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER UNIGRIP	ANALOG	LAB SCANBODY
41.320.090.01-2	-	43.618.201.01-2	18	40.320.008.03-2	43.601.108.01-2	22.613.027.01-2	30.413.002.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES



STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0027	LAB SCANBODY	DAS_C_E_0027
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0027	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0027
	DAS_I_12_0027		DAS_C_I_12_0027

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0028

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c
0,3 mm				mm				mm				mm			
R	31.324.028.01-2	35°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.314.028.01-2			-			-		-						

DYNAMIC 3TIBASE®			
GINGIVAL HEIGHT		α _s	α _s
0,3 mm		CH=5mm	CH= 7mm
R	-	-	-
NR	-		

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}
52.410.109.01-2	10	50.314.028.01-2	43.621.410.01-2	34.614.028.01-2	-	-	33.390.958.01-2	3	30°
			43.624.410.01-2				33.490.958.01-2	4	
52.412.109.01-2	12		43.630.410.01-2				33.690.958.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER UNIGRIP	ANALOG	LAB SCANBODY
41.320.090.01-2	-	43.618.201.01-2	18	40.320.008.03-2	43.601.108.01-2	22.614.028.01-2	30.413.002.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES



STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0028	LAB SCANBODY	DAS_C_E_0028
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0028	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0028
	DAS_I_12_0028		DAS_C_I_12_0028

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0029

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c
1,2 mm				2 mm				3 mm				4 mm			
R	31.322.029.01-2	37°	23°	31.322.029.02-2	25°	15°	31.322.029.03-2	20	25	31.322.029.04-2	15°	25°	-	-	-
NR	31.312.029.01-2			31.312.029.02-2			31.312.029.03-2			31.312.029.04-2			-		

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL			SCANALOG	
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT- CHROME		α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}	
52.410.103.01-2	10	50.312.029.01-2 50.312.029.03-2 (IG=3mm)	43.621.410.01-2	34.613.029.01-2	-	-	33.345.804.01-2	3	20°	23.412.029.01-2	
			43.624.410.01-2				33.445.804.01-2	4			
52.412.103.01-2	12		43.630.410.01-2				33.645.804.01-2	6			

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.20	ANALOG	LAB SCANBODY
41.316.094.01-2	41.316.132.01-2	43.618.201.01-2	18	40.316.003.02-2	43.601.103.02-2	-	30.412.001.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				


LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0029	LAB SCANBODY	DAS_C_E_0029
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0029 DAS_IG_10_0029	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0029 DAS_C_IG_10_0029
	DAS_I_12_0029 DAS_IG_12_0029		DAS_C_I_12_0029 DAS_C_IG_12_0029
	SCANALOG	SCANALOG	DAS_C_SA_0029

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height
IG = Adaptor (3mm)

α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

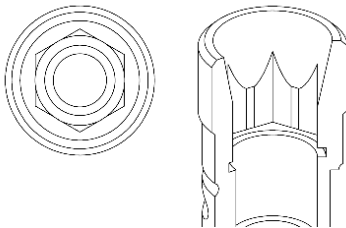

COMPATIBLE with 0030

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c
1,1 mm				2 mm				3 mm				4 mm			
R	31.323.030.01-2	42°	25°	31.323.030.02-2	25°	15°	31.323.030.03-2	20°	30°	31.323.030.04-2	15°	30°	-	-	-
NR	31.313.030.01-2			31.313.030.02-2			31.313.030.03-2			31.313.030.04-2			-		

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
		CH=5mm	CH= 7mm	CH= 9mm
R	31.323.030.21-2	25°	20°	10°
NR	31.313.030.21-2			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL			SCANALOG
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT- CHROME		α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}
52.408.101.01-2	8	50.313.030.01-2 50.313.030.03-2 (IG=3mm)	43.621.410.01-2	34.613.030.01-2	32.213.030.02-2		25°	33.345.808.01-2	3	30°
52.410.101.01-2	10		43.624.410.01-2					33.445.808.01-2	4	
52.412.101.01-2	12		43.630.410.01-2					33.645.808.01-2	6	
										23.413.030.01-2

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.20	ANALOG	LAB SCANBODY
41.320.079.01-2	41.320.125.01-2	43.618.201.01-2	18	40.320.003.04-2	43.601.103.02-2	-	30.413.002.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				


LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0030	LAB SCANBODY	DAS_C_E_0030
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_8_0030 DAS_IG_8_0030	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_8_0030 DAS_C_IG_8_0030
	DAS_I_10_0030 DAS_IG_10_0030		DAS_C_I_10_0030 DAS_C_IG_10_0030
	DAS_I_12_0030 DAS_IG_12_0030		DAS_C_I_12_0030 DAS_C_IG_12_0030
SCANALOG	DAS_SA_0030	SCANALOG	DAS_C_SA_0030

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height
IG = Adaptor (3mm)

α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

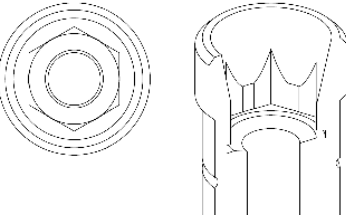

COMPATIBLE with 0033

STANDARD DYNAMIC TIBASE®													
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT	
1,3 mm				2 mm				3mm				4mm	
R	31.322.033.01-2	38°	18°	31.322.033.02-2	20°	14°	15°	31.322.033.03-2	25°	15°	25°	-	-
NR	31.312.033.01-2			31.312.033.02-2				31.312.033.03-2				-	

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
1,3 mm		CH=5mm	CH= 7mm	CH= 9mm
R	31.322.033.21-2	25°	20°	10°
NR	31.312.033.21-2			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME		DYNAMIC MILLING TOOL	SHANK	α _{di}
52.408.106.01-2	8	50.312.033.01-2	43.621.410.01-2	34.612.033.01-2	32.212.033.02-2	25°	33.315.804.01-2	3	25°
52.410.106.01-2	10		43.624.410.01-2				33.415.804.01-2	4	
52.412.106.01-2	12		43.630.410.01-2 (IG=3mm)				33.615.804.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER TORX T6	LAB SCANBODY	
41.316.078.01-2	41.316.124.01-2	43.618.201.01-2	18	40.316.007.01-2	43.601.107.01-2	22.612.033.01-2	30.412.001.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

COMPATIBLE with 0035

STANDARD DYNAMIC TIBASE®													
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT	
1,1 mm				2 mm				3 mm				4 mm	
R	31.323.035.01-2	39°	18°	31.323.035.02-2	20°	14°	15°	31.323.035.03-2	30°	15°	30°	-	-
NR	31.313.035.01-2			31.313.035.02-2				31.313.035.03-2				-	

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
1,1 mm		CH=5mm	CH= 7mm	CH= 9mm
R	31.323.035.21-2	25°	20°	10°
NR	31.313.035.21-2			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL			SCANALOG
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME		DYNAMIC MILLING TOOL	SHANK	α _{di}	
52.410.107.01-2	10	50.313.035.01-2	43.621.410.01-2	34.613.035.01-2	32.213.035.02-2	25°	33.315.804.01-2	3	25°	23.413.035.01-2
			43.624.410.01-2				33.415.804.01-2	4		
52.412.107.01-2	12		43.630.410.01-2 (IG=3mm)				33.615.804.01-2	6		

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER TORX T6	LAB SCANBODY	
41.316.078.01-2	41.316.124.01-2	43.618.201.01-2	18	40.316.007.01-2	43.601.107.01-2	22.613.035.01-2	30.413.002.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

COMPATIBLE with 0037

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c
0,6 mm				mm			mm			mm			mm		
R	31.323.037.01-2	45°	25°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.037.01-2			-			-			-			-		

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL			SCANALOG	
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT- CHROME		α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}	
52.410.110.01-2	10	50.313.037.01-2 50.313.037.04-2 (IG=3mm)	43.621.410.01-2	34.613.037.01-2	32.213.037.02-2	30°	33.315.708.01-2	3	30°	23.413.037.01-2	
			43.624.410.01-2				33.415.708.01-2	4			
52.412.110.01-2	12		43.630.410.01-2				33.615.708.01-2	6			



DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER TORX T6				
41.320.067.01-2	-	43.618.201.01-2	18	40.320.007.01-2	43.601.107.01-2	22.613.037.01-2	30.413.004.01-2		
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0037	LAB SCANBODY	DAS_C_E_0037
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0037 DAS_IG_10_0037	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0037 DAS_C_IG_10_0037
	DAS_I_12_003 DAS_IG_12_0037		DAS_C_I_12_0037 DAS_C_IG_12_0037
SCANALOG	DAS_SA_0037	SCANALOG	DAS_C_SA_0037

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height
IG = Adaptor (3mm)
α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0038

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c
0,7 mm				mm			mm			mm			mm		
R	31.322.038.01-2	45°	29°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.312.038.01-2			-			-			-			-		

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
0,7 mm		CH=5mm	CH= 7mm	CH= 9mm
R	31.322.038.21-2	30°	25°	10°
NR	31.312.038.21-2			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT- CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}
52.410.103.01-2	10	50.312.038.01-2	43.621.410.01-2	34.612.038.01-2	-	-	33.345.804.01-2	3	25°
			43.624.410.01-2				33.445.804.01-2	4	
52.412.103.01-2	12		43.630.410.01-2				33.645.804.01-2	6	



DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.25				
41.316.081.01-2	-	43.618.201.01-2	18	40.316.004.02-2	43.601.104.01-2	22.613.037.01-2	30.413.004.01-2		
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0038	LAB SCANBODY	DAS_C_E_0038
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0038	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0038
	DAS_I_12_0038		DAS_C_I_12_0038

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height
α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0039

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c
0,7 mm				mm				mm				mm			
R	31.323.039.01-2	45°	29°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.039.01-2			-			-			-		-			

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	α _s	α _s	α _s
	0,7 mm	CH=5mm	CH= 7mm	CH= 9mm
R	31.323.039.21-2	30°	25°	10°
NR	31.313.039.21-2			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}
52.410.114.01-2	10	50.313.039.01-2	43.621.410.01-2	34.613.039.01-2	-	-	33.345.856.01-2	3	25°
			43.624.410.01-2				33.445.856.01-2	4	
52.412.114.01-2	12		43.630.410.01-2				33.645.856.01-2	6	


DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.25	ANALOG	LAB SCANBODY
41.316.081.01-2	-	43.618.201.01-2	18	40.316.004.02-2	43.601.104.01-2	-	30.413.002.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0039
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0039
	DAS_I_12_0039
CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_C_E_0039
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0039
	DAS_C_I_12_0039

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

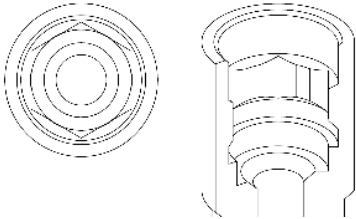

COMPATIBLE with 0040

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c
	0,6 mm			1,5 mm			3 mm			4 mm			5 mm		
R	31.322.040.01-2	45°	30°	31.322.040.02-2	25°	25°	31.322.040.03-2	20°	30°	31.322.040.04-2	15°	30°	31.322.040.05-2	10°	23°
NR	31.312.040.01-2			31.312.040.02-2			31.312.040.03-2			31.312.040.04-2			31.312.040.05-2		
NR (Friction-Fit)	31.312.042.01-2			-			-			-			-		

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	α _s	α _s	α _s
	0,6 mm	CH=5mm	CH= 7mm	CH= 9mm
R	31.322.040.21-2	25°	20°	10°
NR	31.312.040.21-2			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL			SCANALOG
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}	
52.408.101.01-2	8	50.312.040.01-2	43.621.410.01-2	34.612.040.01-2	32.212.040.02-2	25°	33.370.716.01-2	3	25°	23.412.040.01-2
52.410.101.01-2	10		43.624.410.01-2				33.470.716.01-2	4		
52.412.101.01-2	12	50.312.040.03-2 (IG=3mm)	43.630.410.01-2				33.670.716.01-2	6		


DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27	ANALOG	LAB SCANBODY
41.317.071.01-2	41.317.106.01-2	43.618.201.01-2	18	40.317.004.01-2	43.601.104.01-2	22.612.040.01-2	30.412.001.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0040
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_8_0040
	DAS_I_10_0040
	DAS_I_12_0040
	DAS_I_8_0040
	DAS_I_10_0040
	DAS_I_12_0040
SCANALOG	DAS_SA_0040
CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_C_E_0040
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_8_0040
	DAS_C_I_10_0040
	DAS_C_I_12_0040
	DAS_C_I_8_0040
	DAS_C_I_10_0040
	DAS_C_I_12_0040
SCANALOG	DAS_C_SA_0040

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height
IG = Adaptor (3mm)

α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

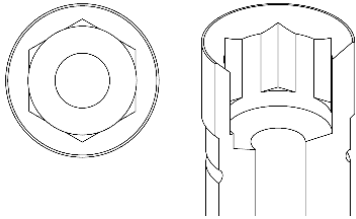

COMPATIBLE with 0040b

STANDARD DYNAMIC TIBASE®													
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT
0,6 mm				1,5 mm			3 mm			mm			5 mm
R	31.322.040.01-2	45°	30°	31.322.040.02-2	25°	25°	31.322.040.03-2	20°	30°	-			31.322.040.05-2
NR	31.312.040.01-2			31.312.040.02-2			31.312.040.03-2			-			31.312.040.05-2

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
0,6 mm		CH=5mm	CH= 7mm	CH= 9mm
R	31.322.040.21-2	25°	20°	10°
NR	31.312.040.21-2			

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}
-	-	-	-	-		32.212.040.02-2	25°	33.370.716.01-2	3	25°
-	-							33.470.716.01-2	4	
-	-							33.670.716.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27	ANALOG	LAB SCANBODY
41.318.071.01-2	-	43.618.201.01-2	18	-	-	-	30.412.001.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				


LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0040	LAB SCANBODY	DAS_C_E_0040
DYNAMIC μSCANBODY (LAB/CLIN)	-	DYNAMIC μSCANBODY (LAB/CLIN)	-
	-		-

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

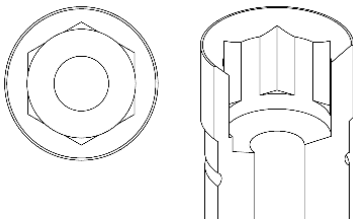

COMPATIBLE with 0041

STANDARD DYNAMIC TIBASE®													
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT
0,4 mm				1,5 mm			mm			mm			mm
R	31.323.041.01-2	45°	30°	31.323.041.02-2	30°	25°	-			-			-
NR	31.313.041.01-2			31.313.041.02-2			-			-			-
NR (Friction-Fit)	31.313.043.01-2			-			-			-			-

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
0,4 mm		CH=5mm	CH= 7mm	CH= 9mm
R	31.323.041.21-2	30°	20°	10°
NR	31.313.041.21-2			

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL			SCANALOG
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}	
52.410.102.01-2	10	50.313.041.01-2	43.621.410.01-2 43.624.410.01-2 43.630.410.01-2	34.613.041.01-2		32.213.041.02-2	30°	33.370.716.01-2	3	30°	23.413.041.01-2
								33.470.716.01-2	4		
52.412.102.01-2	12	50.313.041.03-2 (IG=3mm)						33.670.716.01-2	6		

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27	ANALOG	LAB SCANBODY
41.317.071.01-2	-	43.618.201.01-2	18	40.317.004.01-2	43.601.104.01-2	22.613.041.01-2	30.413.002.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				


LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0041	LAB SCANBODY	DAS_C_E_0041
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0041 DAS_IG_10_0041	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0041 DAS_C_IG_10_0041
	DAS_I_12_0041 DAS_IG_12_0041		DAS_C_I_12_0041 DAS_C_IG_12_0041
SCANALOG	DAS_SA_0041	SCANALOG	DAS_C_SA_0041

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height
IG = Adaptor (3mm)

α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

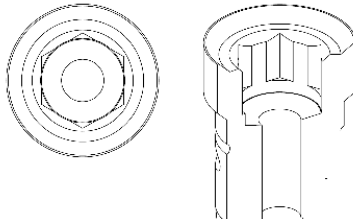

COMPATIBLE with 0041b

STANDARD DYNAMIC TIBASE®													
	GINGIVAL HEIGHT 0,4 mm	α _s	α _c	GINGIVAL HEIGHT 1,5 mm	α _s	α _c	GINGIVAL HEIGHT mm	α _s	α _c	GINGIVAL HEIGHT mm	α _s	α _c	GINGIVAL HEIGHT mm
R	31.323.041.01-2	45°	30°	31.323.041.02-2	30°	25°	-	-	-	-	-	-	-
NR	31.313.041.01-2			31.313.041.02-2			-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT 0,4 mm	α _s CH=5mm	α _s CH= 7mm	α _s CH= 9mm
R	31.323.041.21-2	30°	20°	10°
NR	31.313.041.21-2			

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL	
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT- CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK α _{di}
-	-	-	-	-		32.013.041.02-2	30°	33.370.716.01-2	3
								33.470.716.01-2	4
-	-							33.670.716.01-2	6

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27	ANALOG	LAB SCANBODY
41.318.071.01-2	-	43.618.201.01-2	18	-	-	-	30.413.002.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0041	LAB SCANBODY	DAS_C_E_0041
DYNAMIC μSCANBODY (LAB/CLIN)	-	DYNAMIC μSCANBODY (LAB/CLIN)	-
	-		-

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

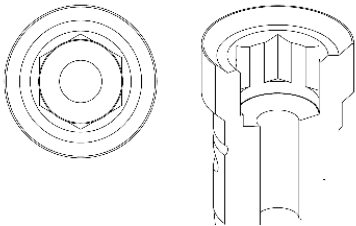

COMPATIBLE with 0044

STANDARD DYNAMIC TIBASE®													
	GINGIVAL HEIGHT 1 mm	α _s	α _c	GINGIVAL HEIGHT mm	α _s	α _c	GINGIVAL HEIGHT mm	α _s	α _c	GINGIVAL HEIGHT mm	α _s	α _c	GINGIVAL HEIGHT mm
R	31.322.044.01-2	42°	23°	-	-	-	-	-	-	-	-	-	-
NR	31.312.044.01-2			-			-			-			-

DYNAMIC 3TIBASE®			
	GINGIVAL HEIGHT 1 mm	α _s CH=5mm	α _s CH= 7mm
R	31.322.044.21-2	25°	20°
NR	-		

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL	
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT- CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK α _{di}
52.410.105.01-2	10	50.312.044.01-2	43.621.410.01-2	34.612.044.01-2		-	-	33.390.716.01-2	3
			43.624.410.01-2					33.490.716.01-2	4
52.412.105.01-2	12		43.630.410.01-2					33.690.716.01-2	6

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.20	ANALOG	LAB SCANBODY
41.318.065.01-2	-	43.618.201.01-2	18	40.318.003.01-2	43.601.103.02-2	-	30.412.001.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0044	LAB SCANBODY	DAS_C_E_0044
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0044	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0044
	DAS_I_12_0044		DAS_C_I_12_0044

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

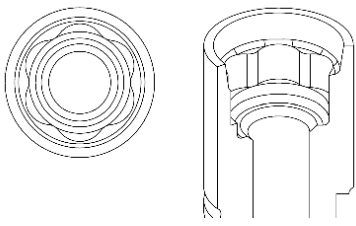

COMPATIBLE with 0045

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c
1 mm				mm				mm				mm			
R	31.323.045.01-2	43°	22°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.045.01-2			-			-		-						

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
1 mm		CH=5mm	CH= 7mm	CH= 9mm
R	31.323.045.21-2	30°	20°	10°
NR	31.313.045.21-2			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}
52.410.118.01-2	10	50.313.045.01-2	43.621.410.01-2	34.613.045.01-2	-	-	33.390.716.01-2	3	30°
			43.624.410.01-2				33.490.716.01-2	4	
52.412.118.01-2	12		43.630.410.01-2				33.690.716.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.20	LAB SCANBODY	
41.318.065.01-2	-	43.618.201.01-2	18	40.318.003.01-2	43.601.103.02-2	-	30.413.002.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0045	LAB SCANBODY	DAS_C_E_0045
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0045	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0045
	DAS_I_12_0045		DAS_C_I_12_0045

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0046

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c
1 mm				mm				mm				mm			
R	31.324.046.01-2	42°	21°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.314.046.01-2			-				-				-			

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
1 mm		CH=5mm	CH= 7mm	CH= 9mm
R	31.324.046.21-2	30°	20°	10°
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}
52.410.125.01-2	10	50.314.046.01-2	43.621.410.01-2	34.614.046.01-2	-	-	33.390.716.01-2	3	30°
			43.624.410.01-2				33.490.716.01-2	4	
52.412.125.01-2	12		43.630.410.01-2				33.690.716.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.20	LAB SCANBODY	
41.318.065.01-2	-	43.618.201.01-2	18	40.318.003.01-2	43.601.103.02-2	-	30.413.002.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES



STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0046	LAB SCANBODY	DAS_C_E_0046
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0046	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0046
	DAS_I_12_0046		DAS_C_I_12_0046

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0047

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c
0,6 mm				mm			mm			mm			mm		
R	31.322.047.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.312.047.01-2			-			-			-			-		

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}
52.410.123.01-2	10	50.312.047.01-2	43.621.410.01-2	34.612.047.01-2	-	-	33.390.716.01-2	3	25°
			43.624.410.01-2				33.490.716.01-2	4	
52.412.123.01-2	12		43.630.410.01-2				33.690.716.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER TORX T6	ANALOG	LAB SCANBODY
41.320.074.01-2	-	43.618.201.01-2	18	40.320.007.02-2	43.601.107.01-2	-	30.412.001.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

COMPATIBLE with 0048

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c
0,6 mm				mm			mm			mm			mm		
R	31.323.048.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.048.01-2			-			-			-			-		

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}
52.410.123.01-2	10	50.312.047.01-2	43.621.410.01-2	34.612.047.01-2	-	-	33.390.716.01-2	3	30°
			43.624.410.01-2				33.490.716.01-2	4	
52.412.123.01-2	12		43.630.410.01-2				33.690.716.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER TORX T6	ANALOG	LAB SCANBODY
41.320.074.01-2	-	43.618.201.01-2	18	40.320.007.02-2	43.601.107.01-2	-	30.413.002.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				



LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0048	LAB SCANBODY	DAS_C_E_0048
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0048	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0048
	DAS_I_12_0048		DAS_C_I_12_0048

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0049

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c
0,6 mm				mm			mm			mm			mm		
R	31.321.049.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.311.049.01-2			-			-			-			-		

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}
52.410.116.01-2	10	50.311.049.01-2	43.621.410.01-2	34.611.049.01-2	-	-	33.325.472.01-2*	3	25°
			43.624.410.01-2				33.425.472.01-2*	4	
52.412.116.01-2	12		43.630.410.01-2				33.625.472.01-2*	6	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.25	ANALOG	LAB SCANBODY
41.314.064.01-2	-	43.618.201.01-2	18	40.314.004.01-2	43.601.104.01-2	-	30.412.001.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

COMPATIBLE with 0050

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c
0,5 mm				1,2 mm			mm			mm			mm		
R	31.323.051.01-2	45°	27°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.051.01-2			-			-			-			-		

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}
52.410.117.01-2	10	50.312.050.01-2	43.621.410.01-2	34.612.050.01-2	-	-	33.335.676.01-2	3	25°
		50.312.050.04-2 (IG=3mm)	43.624.410.01-2				33.435.676.01-2	4	
52.412.117.01-2	12		43.630.410.01-2				33.635.676.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.25	ANALOG	LAB SCANBODY
41.318.064.01-2	-	43.618.201.01-2	18	40.318.004.03-2	43.601.104.01-2	-	30.412.001.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

COMPATIBLE with 0051

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c
0,5 mm				mm			mm			mm			mm		
R	31.323.051.01-2	45°	25°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.051.01-2			-			-			-			-		

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}
52.410.118.01-2	10	50.313.051.01-2 50.313.051.04-2 (IG=3mm)	43.621.410.01-2	34.613.051.01-2	-	-	33.335.676.01-2	3	25°
			43.624.410.01-2				33.435.676.01-2	4	
52.412.118.01-2	12		43.630.410.01-2				33.635.676.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.25	ANALOG	LAB SCANBODY
41.318.064.01-2	-	43.618.201.01-2	18	40.318.004.03-2	43.601.104.01-2	-	30.412.001.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

COMPATIBLE with 0052

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c
0,3 mm				mm			mm			mm			mm		
R	31.324.052.01-2	45°	27°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.314.052.01-2			-			-			-			-		

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}
52.410.102.01-2	10	50.314.052.01-2	43.621.410.01-2	34.614.052.01-2	-	-	33.335.676.01-2	3	30°
			43.624.410.01-2				33.435.676.01-2	4	
52.412.102.01-2	12		43.630.410.01-2				33.635.676.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.25	ANALOG	LAB SCANBODY
41.318.064.01-2	-	43.618.201.01-2	18	40.318.004.03-2	43.601.104.01-2	-	30.413.002.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				



LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0052	LAB SCANBODY	DAS_C_E_0052
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0052	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0052
	DAS_I_12_0052		DAS_C_I_12_0052

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0054

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT	α_s	α_c	GINGIVAL HEIGHT	α_s	α_c	GINGIVAL HEIGHT	α_s	α_c	GINGIVAL HEIGHT	α_s	α_c
0,6 mm				mm			mm			mm			mm		
R	31.323.054.01-2	45°	25°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.054.01-2			-			-			-			-		

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α_s	α_s	α_s
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
52.410.119.01-2	10	50.314.054.01-2	43.621.410.01-2	34.614.054.01-2	-	-	33.345.856.01-2	3	30°
			43.624.410.01-2				33.445.856.01-2	4	
52.412.119.01-2	12		43.630.410.01-2				33.645.856.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER	ANALOG	LAB SCANBODY
41.318.067.01-2	-	43.618.201.01-2	18	40.318.012.01-2	-	-	30.413.002.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				


LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0054	LAB SCANBODY	DAS_C_I_0054
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0054	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0054
	DAS_I_12_0054		DAS_C_I_12_0054

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

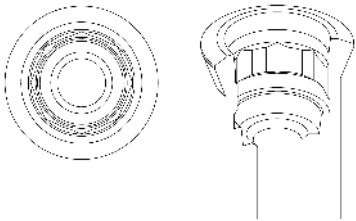

COMPATIBLE with 0057

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c
0,5 mm				mm			mm			mm			mm		
R	31.324.057.01-2	45°	27°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.314.057.01-2			-			-			-			-		

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α_s	α_s	α_s
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
52.408.101.01-2	8	50.314.057.01-2	43.621.410.01-2	34.614.057.01-2	-	-	33.390.805.01-2	3	30°
52.410.101.01-2	10		43.624.410.01-2				33.490.805.01-2	4	
52.412.101.01-2	12		43.630.410.01-2				33.690.805.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.20	ANALOG	LAB SCANBODY
41.316.084.01-2	-	43.618.201.01-2	18	40.316.003.01-2	43.601.103.02-2	22.614.057.01-2	30.414.003.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				


LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0057	LAB SCANBODY	DAS_C_E_0057
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_8_0057	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_8_0057
	DAS_I_10_0057		DAS_C_I_10_0057
	DAS_I_12_0057		DAS_C_I_12_0057

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

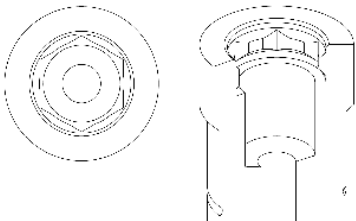

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c
0,5 mm				mm			mm			mm			mm		
R	31.324.058.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.314.058.01-2			-			-			-			-		

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α_s	α_s	α_s
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
52.410.118.01-2	10	50.314.058.01-2	43.621.410.01-2	34.614.058.01-2	-	-	33.390.716.01-2	3	30°
			43.624.410.01-2				33.490.716.01-2	4	
52.412.118.01-2	12		43.630.410.01-2				33.690.716.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.20		LAB SCANBODY
41.320.047.01-2	-	43.618.201.01-2	18	40.320.003.01-2	43.601.103.02-2	22.614.058.01-2	30.414.003.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				


LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0058	LAB SCANBODY	DAS_C_E_0058
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0058	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0058
	DAS_I_12_0058		DAS_C_I_12_0058

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

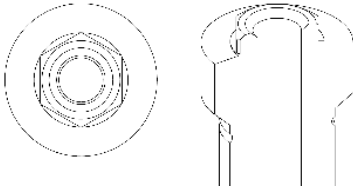

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c
0,7 mm				mm			mm			mm			mm		
R	31.324.059.01-2	45°	27°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.314.059.01-2			-			-			-			-		

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α_s	α_s	α_s
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
52.410.115.01-2	10	50.313.010.01-2	43.621.410.01-2	34.614.059.01-2	-	-	33.390.716.01-2	3	25
			43.624.410.01-2				33.490.716.01-2	4	
52.412.115.01-2	12		43.630.410.01-2 (IG=3mm)				33.690.716.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.20		LAB SCANBODY
41.318.065.01-2	-	43.618.201.01-2	18	40.318.003.01-2	43.601.103.02-2	22.614.059.01-2	30.414.003.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				


LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0059	LAB SCANBODY	DAS_C_E_0059
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0059 DAS_IG_10_0059	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0059 DAS_C_IG_10_0059
	DAS_I_12_0059 DAS_IG_12_0059		DAS_C_I_12_0059 DAS_C_IG_12_0059

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height
IG = Adaptor 3mm

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

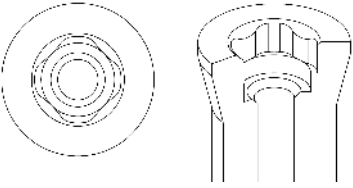

COMPATIBLE with 0060

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c
0,5 mm				mm			mm			mm			mm		
R	31.324.060.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.314.060.01-2			-			-			-			-		

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α_s	α_s	α_s
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
52.410.122.01-2	10	50.314.060.01-2	43.621.410.01-2	34.614.060.01-2	-	-	33.390.716.01-2	3	30°
			43.624.410.01-2				33.490.716.01-2	4	
52.412.122.01-2	12		43.630.410.01-2				33.690.716.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.20		LAB SCANBODY
41.320.060.01-2	-	43.618.201.01-2	18	40.320.003.02-2	43.601.103.02-2	22.614.060.01-2	30.415.007.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES



STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0060	LAB SCANBODY	DAS_C_E_0060
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0060	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0060
	DAS_I_12_0060		DAS_C_I_12_0060

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0061

STANDARD DYNAMIC TIBASE®																	
GINGIVAL HEIGHT		α_s		α_c		GINGIVAL HEIGHT		α_s		α_c		GINGIVAL HEIGHT		α_s		α_c	
0,6 mm				mm				mm				mm				mm	
R	31.324.061.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.314.061.01-2			-			-			-			-				

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α_s	α_s	α_s
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
52.410.125.01-2	10	50.314.061.01-2	43.621.410.01-2	34.614.061.01-2	-	-	33.390.958.01-2	3	30°
			43.624.410.01-2				33.490.958.01-2	4	
52.412.125.01-2	12		43.630.410.01-2				33.690.958.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER UNIGRIP		LAB SCANBODY
41.325.067.01-2	-	43.618.201.01-2	18	40.325.008.01-2	43.601.108.01-2	22.614.061.01-2	30.415.007.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES



STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0061	LAB SCANBODY	DAS_C_E_0061
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0061	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0061
	DAS_I_12_0061		DAS_C_I_12_0061

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0066

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c
0,6 mm				mm				mm				mm			
R	31.323.066.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	-			-			-		-						

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α_s	α_s	α_s
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
-	-	-	-	-	-	-	-	-	-	-
								-	-	
-	-							-	-	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER	ANALOG	LAB SCANBODY
41.314.039.01-2	-	43.618.201.01-2	18	-	-	22.613.066.01-2	30.412.001.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES



STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0066	LAB SCANBODY	DAS_C_E_0066
DYNAMIC μSCANBODY (LAB/CLIN)	-	DYNAMIC μSCANBODY (LAB/CLIN)	-
	-		-

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0074

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
0,6 mm				mm				mm				mm			
R	31.323.074.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.074.01-2			-				-				-			

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α_s	α_s	α_s
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL			SCANALOG
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}	
52.410.110.01-2	10	50.313.074.01-2	43.621.410.01-2	34.613.074.01-2	-	-	-	33.330.708.01-2	3	30°	23.413.074.01-2
			43.624.410.01-2					33.430.708.01-2	4		
52.412.110.01-2	12		43.630.410.01-2					33.630.708.01-2	6		

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Sq. 1.30	ANALOG	LAB SCANBODY
41.320.044.01-2	-	43.618.201.01-2	18	40.320.007.04-2	43.601.102.01-2	22.613.074.01-2	30.415.007.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0074	LAB SCANBODY	DAS_C_E_0074
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0074	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0074
	DAS_I_12_0074		DAS_C_I_12_0074
SCANALOG	DAS_SA_0074	SCANALOG	DAS_C_SA_0074

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0075

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c
1 mm		42°	24°	2 mm		25°	15°	mm		-	-	mm		-	-
R	31.322.075.01-2			31.322.075.02-2				-	-			-	-		
NR	-			-				-	-			-	-		

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α_s	α_s	α_s
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
52.410.105.01-2	10	50.312.075.01-2	43.621.410.01-2	34.612.075.01-2	-	-	33.330.734.01-2	3	25°
			43.624.410.01-2				33.430.734.01-2	4	
52.412.105.01-2	12		43.630.410.01-2				33.630.734.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.00		LAB SCANBODY
41.318.077.01-2	-	43.618.201.01-2	18	40.318.013.01-2	-	22.612.075.01-2	30.412.001.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0075	LAB SCANBODY	DAS_C_E_0075
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0075	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0075
	DAS_I_12_0075		DAS_C_I_12_0075

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

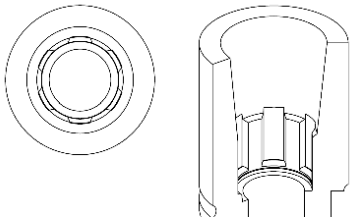

COMPATIBLE with 0080

STANDARD DYNAMIC TIBASE®																	
GINGIVAL HEIGHT		α_s		α_c		GINGIVAL HEIGHT		α_s		α_c		GINGIVAL HEIGHT		α_s		α_c	
0,4 mm				mm						mm						mm	
R	31.324.080.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-	-	
NR	31.314.080.01-2			-			-			-		-			-		

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α_s	α_s	α_s
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
52.410.124.01-2	10	50.314.080.01-2	43.621.410.01-2	34.614.080.01-2	-	-	33.370.716.01-2	3	30°
			43.624.410.01-2				33.470.716.01-2	4	
52.412.124.01-2	12		43.630.410.01-2				33.670.716.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27		LAB SCANBODY
41.317.071.01-2	-	43.618.201.01-2	18	40.317.004.01-2	43.601.104.01-2	22.614.080.01-2	30.414.003.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0080	LAB SCANBODY	DAS_C_E_0080
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0080	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0080
	DAS_I_12_0080		DAS_C_I_12_0080

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

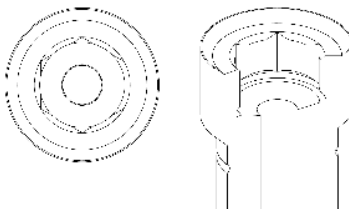

COMPATIBLE with 0081

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c
0,4 mm				mm			mm			mm			mm		
R	31.325.081.01-2	41°	18°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.315.081.01-2			-			-			-			-		

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α_s	α_s	α_s
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
52.410.126.01-2	10	50.315.081.01-2	43.621.410.01-2	34.615.081.01-2	-	-	33.335.676.01-2	3	30°
			43.624.410.01-2				33.435.676.01-2	4	
52.412.126.01-2	12		43.630.410.01-2				33.635.676.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.25	ANALOG	LAB SCANBODY
41.318.064.01-2	-	43.618.201.01-2	18	40.318.004.03-2	43.601.104.01-2	-	30.414.003.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				


LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0081	LAB SCANBODY	DAS_C_E_0081
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0081	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0081
	DAS_I_12_0081		DAS_C_I_12_0081

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

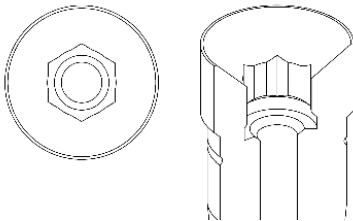

COMPATIBLE with 0082

STANDARD DYNAMIC TIBASE®																	
GINGIVAL HEIGHT		α_s		α_c		GINGIVAL HEIGHT		α_s		α_c		GINGIVAL HEIGHT		α_s		α_c	
1,2 mm				mm						mm						mm	
R	31.322.082.01-2	45°	25°	-	-	-	-	-	-	-	-	-	-	-	-		
NR	31.312.082.01-2			-			-			-			-				

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α_s	α_s	α_s
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
52.410.105.01-2	10	50.312.082.01-2	43.621.410.01-2	34.612.082.01-2	-	-	33.345.804.01-2	3	25°
			43.624.410.01-2				33.445.804.01-2	4	
52.412.105.01-2	12		43.630.410.01-2				33.645.804.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER -	ANALOG	LAB SCANBODY
41.316.074.01-2	-	43.618.201.01-2	18	40.316.012.01-2	-	-	30.412.001.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				


LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0082	LAB SCANBODY	DAS_C_E_0082
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0082	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0082
	DAS_I_12_0082		DAS_C_I_12_0082

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

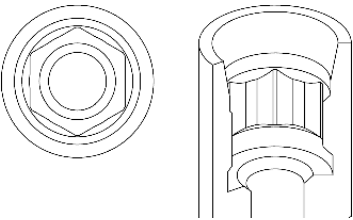

COMPATIBLE with 0083

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c
1,2 mm				mm			mm			mm			mm		
R	31.323.083.01-2	45°	25°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.083.01-2			-			-			-			-		

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α_s	α_s	α_s
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
52.410.103.01-2	10	50.313.083.01-2	43.621.410.01-2	34.613.083.01-2		-	-	33.345.856.01-2	3	30°
			43.624.410.01-2					33.445.856.01-2	4	
52.412.103.01-2	12		43.630.410.01-2					33.645.856.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER	ANALOG	LAB SCANBODY
41.318.076.01-2	-	43.618.201.01-2	18	40.318.012.02-2	-	-	30.413.002.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES



STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0083	LAB SCANBODY	DAS_C_E_0083
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0083	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0083
	DAS_I_12_0083		DAS_C_I_12_0083

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0084

STANDARD DYNAMIC TIBASE®																	
GINGIVAL HEIGHT		α_s		α_c		GINGIVAL HEIGHT		α_s		α_c		GINGIVAL HEIGHT		α_s		α_c	
1,2 mm				mm						mm						mm	
R	31.321.084.01-2	30°	-	-	-	-	-	-	-	-	-	-	-	-	-		
NR	31.311.084.01-2			-			-			-			-				

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α_s	α_s	α_s
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
-	-	-	-	-		-	-	-	-	-
								-	-	
-	-							-	-	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER	ANALOG	LAB SCANBODY
41.314.076.01-2	-	43.618.201.01-2	18	40.314.003.03-2	Star 1.50 43.601.103.02-2	-	30.410.006.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES



STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0084	LAB SCANBODY	-
DYNAMIC μSCANBODY (LAB/CLIN)	-	DYNAMIC μSCANBODY (LAB/CLIN)	-
	-		-

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0085

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c
0,3 mm				mm			mm			mm			mm		
R	31.324.085.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.314.085.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}
52.410.117.01-2	10	50.314.085.01-2	43.621.410.01-2	34.614.085.01-2	-	-	33.345.856.01-2	3	25°
			43.624.410.01-2				33.445.856.01-2	4	
52.412.117.01-2	12		43.630.410.01-2				33.645.856.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.25	ANALOG	LAB SCANBODY
41.316.081.01-2	-	43.618.201.01-2	18	40.316.004.02-2	43.601.104.01-2	-	30.413.002.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES



STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0085	LAB SCANBODY	DAS_C_E_0085
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0085	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0085
	DAS_I_12_0085		DAS_C_I_12_0085

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0086

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c
1 mm				mm			mm			mm			mm		
R	31.325.086.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.315.086.01-2			-			-			-			-		

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}
-	-	-	-	-	-	-	-	-	-
							-	-	
-	-						-	-	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.25	ANALOG	LAB SCANBODY
41.316.081.01-2	-	43.618.201.01-2	18	40.316.004.02-2	43.601.104.01-2	-	30.415.007.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0086	LAB SCANBODY	DAS_C_E_0086
DYNAMIC μSCANBODY (LAB/CLIN)	-	DYNAMIC μSCANBODY (LAB/CLIN)	-
	-		-

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0090

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c
1 mm				mm			mm			mm			mm		
R	31.321.090.01-2	45°	24°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.311.090.01-2			-			-			-			-		

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α_s	α_s	α_s
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
52.410.128.01-2	10	50.311.090.01-2	43.621.415.01-2-	34.611.090.01-2		-	-	33.325.472.01-2*	3	25°
								33.425.472.01-2*	4	
-	-							33.625.472.01-2*	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27		LAB SCANBODY
41.314.074.01-2	-	43.618.201.01-2	18	40.314.005.01-2	43.601.105.01-2	-	30.410.006.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

COMPATIBLE with 0091

STANDARD DYNAMIC TIBASE®																	
GINGIVAL HEIGHT		α_s		α_c		GINGIVAL HEIGHT		α_s		α_c		GINGIVAL HEIGHT		α_s		α_c	
1,2 mm				mm								mm					
R	31.324.091.01-2	38°	18°	-	-	-	-	-	-	-	-	-	-	-	-		
NR	31.314.091.01-2			-			-			-			-				

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α_s	α_s	α_s
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
52.410.102.01-2	10	50.314.091.01-2	43.621.410.01-2 43.624.410.01-2 43.630.410.01-2	34.614.091.01-2		-	-	33.390.958.01-2	3	30°
								33.490.958.01-2	4	
52.412.102.01-2	12							33.690.958.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27		LAB SCANBODY
41.320.082.01-2	-	43.618.201.01-2	18	40.320.005.01-2	43.601.105.01-2	22.614.091.01-2	30.413.002.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				


LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0091	LAB SCANBODY	DAS_C_E_0091
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0091	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0091
	DAS_I_12_0091		DAS_C_I_12_0091

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0092

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c
1 mm				mm				mm				mm			
R	31.325.092.01-2	45°	25°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.315.092.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α_s	α_s	α_s
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
52.410.129.01-2	10	50.315.092.01-2	43.621.410.01-2	34.615.092.01-2	-	-	33.390.958.01-2	3	30°
			43.624.410.01-2				33.490.958.01-2	4	
52.412.129.01-2	12		43.630.410.01-2				33.690.958.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27	ANALOG	LAB SCANBODY
41.320.082.01-2	-	43.618.201.01-2	18	40.320.005.01-2	43.601.105.01-2	22.615.092.01-2	30.415.007.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0092	LAB SCANBODY	DAS_C_E_0092
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0092	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0092
	DAS_I_12_0092		DAS_C_I_12_0092

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

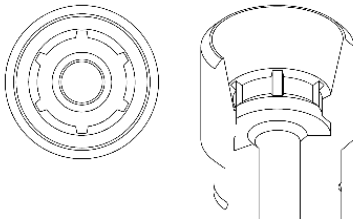

COMPATIBLE with 0096

STANDARD DYNAMIC TIBASE®																	
GINGIVAL HEIGHT		α_s		α_c		GINGIVAL HEIGHT		α_s		α_c		GINGIVAL HEIGHT		α_s		α_c	
0,6 mm				mm						mm						mm	
R	31.324.096.01-2	45°	30°	-		-		-		-		-		-		-	
NR	31.314.096.01-2			-		-		-		-		-		-		-	

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α_s	α_s	α_s
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL			SCANALOG
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}	
52.410.110.01-2	10	50.314.096.01-2	43.621.410.01-2	34.614.096.01-2	-	-	33.315.708.01-2	3	30°	23.414.096.01-2
			43.624.410.01-2				33.415.708.01-2	4		
52.412.110.01-2	12		43.630.410.01-2				33.615.708.01-2	6		

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER TORX T6	ANALOG	LAB SCANBODY
41.320.067.01-2	-	43.618.201.01-2	18	40.320.007.01-2	43.601.107.01-2	22.614.096.01-2	30.414.008.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0096	LAB SCANBODY	DAS_C_E_0096
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0096	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0096
	DAS_I_12_0096		DAS_C_I_12_0096
SCANALOG	DAS_SA_0096	SCANALOG	DAS_C_SA_0096

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

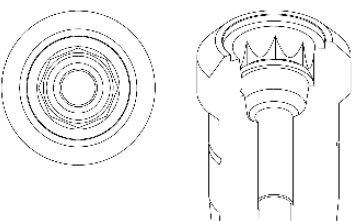

COMPATIBLE with 0101

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c
0,5 mm				mm			mm			mm			mm		
R	31.323.101.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	-			-			-			-			-		

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL			SCANALOG
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT- CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}	
54.409.133.01-2	9	50.313.101.01-2	43.621.410.01-2	34.613.101.01-2	-	-	-	-	-	23.413.101.01-2
			43.624.410.01-2				-	-		
-	-		43.630.410.01-2				-	-		

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER TORX T6	LAB SCANBODY	
41.314.043.01-2	-	43.618.201.01-2	18	40.314.007.01-2	43.601.107.01-2	-	30.413.005.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0101	LAB SCANBODY	DAS_C_E_0101
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_9_0101	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_9_101
	-		-
SCANALOG	DAS_SA_0101	SCANALOG	DAS_C_SA_0101

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0102

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c
1,8 mm				mm			mm			mm			mm		
R	31.322.102.01-2	38°	18°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.312.102.01-2			-			-			-			-		

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
1,8 mm		CH=5mm	CH= 7mm	CH= 9mm
R	31.322.102.21-2	25°	15°	10°
NR	31.312.102.21-2			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT- CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}
52.410.128.01-2	10	50.312.102.03-2 (IG=3mm)	43.621.415.01-2	34.612.102.01-2	-	-	-	-	-
							-	-	
52.412.128.01-2	12						-	-	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27	LAB SCANBODY	
41.317.065.01-2	-	43.618.201.01-2	18	40.317.005.02-2	43.601.105.01-2	-	30.412.001.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES



STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0102	LAB SCANBODY	DAS_C_E_0102
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_IG_10_0102	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_IG_10_0102
	DAS_IG_12_0102		DAS_C_IG_12_0102

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height
IG = Adaptor (3mm)

α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0109

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c
1,2 mm				mm			mm			mm			mm		
R	31.322.109.01-2	45°	29°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.312.109.01-2			-			-			-			-		

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}
52.410.128.01-2	10	50.312.109.01-2	43.621.415.01-2	34.612.109.01-2	-	-	33.360.754.01-2*	3	25°
							33.460.754.01-2*	4	
52.412.128.01-2	12						33.660.754.01-2*	6	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27	ANALOG	LAB SCANBODY
41.314.070.01-2	-	43.618.201.01-2	18	40.314.005.02-2	43.601.105.01-2	-	30.412.001.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES



STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0109	LAB SCANBODY	DAS_C_E_0109
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0109	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0109
	DAS_I_12_0109		DAS_C_I_12_0109

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0110

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c
0,4 mm				mm			mm			mm			mm		
R	31.320.110.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.310.110.01-2			-			-			-			-		

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}
52.410.117.01-2	10	50.310.110.04-2 IG=3mm	43.621.410.01-2 43.624.410.01-2 43.630.410.01-2	34.610.110.01-2	-	-	33.360.756.01-2	3	20°
							33.460.756.01-2	4	
52.412.117.01-2	12						33.660.756.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER TORX T6	ANALOG	LAB SCANBODY
41.318.083.01-2	-	43.618.201.01-2	18	-	-	-	30.410.006.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES



STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0110	LAB SCANBODY	DAS_C_E_0110
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_IG_10_0110	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_IG_10_0110
	DAS_IG_12_0110		DAS_C_IG_12_0110

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height
IG = Adaptor (3mm)

α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0111

STANDARD DYNAMIC TIBASE®																
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	
0,4 mm		45°	30°	mm	-	-	mm	-	-	mm	-	-	mm	-	-	
R	31.323.111.01-2			-			-			-			-			-
NR	31.313.111.01-2			-			-			-			-			-

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}
52.410.117.01-2	10	50.310.110.04-2 IG=3mm	43.621.410.01-2 43.624.410.01-2 43.630.410.01-2	34.610.110.01-2	-	-	33.360.756.01-2	3	20°
							33.460.756.01-2	4	
52.412.117.01-2	12						33.660.756.01-2	6	


DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER TORX T6	ANALOG	LAB SCANBODY
41.318.083.01-2	-	43.618.201.01-2	18	-	-	-	30.413.002.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0111	LAB SCANBODY	DAS_C_E_0111
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_IG_10_0111	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_IG_10_0111
	DAS_IG_12_0111		DAS_C_IG_12_0111

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height
IG = Adaptor (3mm)
α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

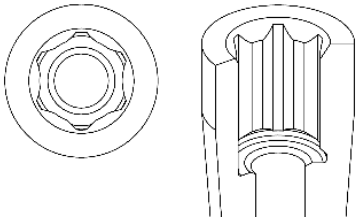

COMPATIBLE with 0120

STANDARD DYNAMIC TIBASE®																	
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c		
1 mm		45°	25°	mm	-	-	mm	-	-	mm	-	-	mm	-	-		
R	31.323.121.01-2			-			-			-			-			-	-
NR	31.313.121.01-2			-			-			-			-			-	-

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}
-	-	-	-	-	-	-	33.360.754.01-2	3	20°
							33.460.754.01-2	4	
-	-						33.660.754.01-2	6	


DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27	ANALOG	LAB SCANBODY
41.316.080.01-2	-	43.618.201.01-2	18	40.316.005.07-2	43.601.105.01-2	-	30.413.002.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0120	LAB SCANBODY	DAS_C_E_0120
DYNAMIC μSCANBODY (LAB/CLIN)	-	DYNAMIC μSCANBODY (LAB/CLIN)	-
	-		-

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height
α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

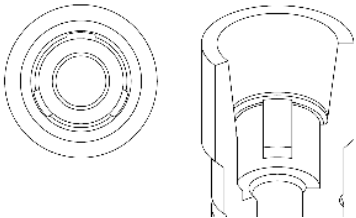

COMPATIBLE with 0121

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c
1 mm				mm				mm				mm			
R	31.323.121.01-2	45°	25°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.121.01-2			-			-		-						

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α_s	α_s	α_s
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
-	-	-	-	-		-	-	33.360.754.01-2	3	20°
								33.460.754.01-2	4	
-	-							33.660.754.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27	ANALOG	LAB SCANBODY
41.316.080.01-2	-	43.618.201.01-2	18	40.316.005.07-2	43.601.105.01-2	-	30.413.002.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0121	LAB SCANBODY	DAS_C_E_0121
DYNAMIC μSCANBODY (LAB/CLIN)	-	DYNAMIC μSCANBODY (LAB/CLIN)	-
	-		-

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

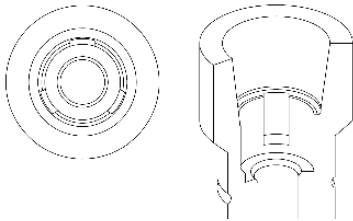

COMPATIBLE with 0124

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
1,4 mm				mm				mm				mm			
R	31.324.124.01-2	42°	19°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.314.124.01-2			-				-				-			

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α_s	α_s	α_s
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
52.410.125.01-2	10	50.314.124.01-2	43.621.410.01-2	34.614.124.01-2		-	-	33.335.758.01-2	3	30°
			43.624.410.01-2					33.435.758.01-2	4	
52.412.125.01-2	12		43.630.410.01-2					33.635.758.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER UNIGRIP	ANALOG	LAB SCANBODY
41.320.075.01-2	-	43.618.201.01-2	18	40.320.008.02-2	43.601.108.01-2	-	30.414.003.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0124	LAB SCANBODY	DAS_C_E_0124
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0124	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0124
	DAS_I_12_0124		DAS_C_I_12_0124

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

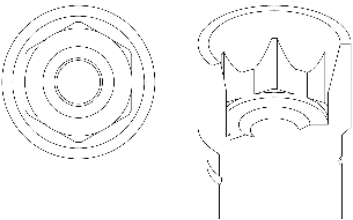

COMPATIBLE with 0125

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT	α_s	α_c	GINGIVAL HEIGHT	α_s	α_c	GINGIVAL HEIGHT	α_s	α_c	GINGIVAL HEIGHT	α_s	α_c
1,1 mm				mm			mm			mm			mm		
R	31.323.125.01-2	42°	20°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.125.01-2			-			-			-			-		

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α_s	α_s	α_s
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
52.410.117.01-2	10	50.313.125.01-2	43.621.410.01-2	34.613.125.01-2		-	-	33.315.804.01-2	3	25°
			43.624.410.01-2					33.415.804.01-2	4	
52.412.117.01-2	12		43.630.410.01-2					33.615.804.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER TORX T6	ANALOG	LAB SCANBODY
41.316.078.01-2	-	43.618.201.01-2	18	40.316.007.01-2	43.601.107.01-2	-	30.413.002.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES



STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0125	LAB SCANBODY	DAS_C_E_0125
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0125	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0125
	DAS_I_12_0125		DAS_C_I_12_0125

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0128

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c
2,5 mm				mm			mm			mm			mm		
R	31.322.128.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	-			-			-			-			-		

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α_s	α_s	α_s
		CH=5mm	CH= 7mm	CH= 9mm
-	-	-	-	-
-	-			

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
-	-	-	-	-		-	-	-	-	-
								-	-	
-	-							-	-	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.20	ANALOG	LAB SCANBODY
41.320.044.01-2	-	43.618.201.01-2	18	40.320.003.05-2	43.601.103.01-2	-	30.413.002.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES



STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0128	LAB SCANBODY	DAS_C_E_0128
DYNAMIC μSCANBODY (LAB/CLIN)	-	DYNAMIC μSCANBODY (LAB/CLIN)	-
	-		-

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0129

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c
0,3 mm				mm				mm				mm			
R	31.325.129.01-2	43°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.315.129.01-2			-			-		-						

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α_s	α_s	α_s
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME		DYNAMIC MILLING TOOL	SHANK	α_{di}
52.410.130.01-2	10	50.315.129.01-2	43.621.410.01-2	34.615.129.01-2	-	-	33.390.958.01-2	3	30°
			43.624.410.01-2				33.490.958.01-2	4	
52.412.130.01-2	12		43.630.410.01-2				33.690.958.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER UNIGRIP	ANALOG	LAB SCANBODY
41.320.090.01-2	-	43.618.201.01-2	18	40.320.008.03-2	43.601.108.01-2	22.615.129.01-2	30.415.007.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES



STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	-	LAB SCANBODY	-
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0129	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0129
	DAS_I_12_0129		DAS_C_I_12_0129

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0130

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
0,5 mm				mm				mm				mm			
R	31.322.130.01-2	30°	29°	-		-	-	-		-	-	-		-	-
NR	31.312.130.01-2			-				-				-			

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α_s	α_s	α_s
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME		DYNAMIC MILLING TOOL	SHANK	α_{di}
-	-	-	-	-	-	-	33.345.804.01-2	3	20°
							33.445.804.01-2	4	
-	-						33.645.804.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27	ANALOG	LAB SCANBODY
41.316.081.01-2	-	43.618.201.01-2	18	40.316.005.08-2	43.601.105.01-2	-	30.412.001.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES



STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0130	LAB SCANBODY	DAS_C_E_0130
DYNAMIC μSCANBODY (LAB/CLIN)	-	DYNAMIC μSCANBODY (LAB/CLIN)	-
	-		-

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c
0,5 mm				mm				mm				mm			
R	31.323.131.01-2	45°	29°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.131.01-2			-			-			-					

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α_s	α_s	α_s
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
-	-	-	-	-		-	-	33.345.804.01-2	3	20°
								33.445.804.01-2	4	
-	-							33.645.804.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27	ANALOG	LAB SCANBODY
41.316.081.01-2	-	43.618.201.01-2	18	40.316.005.08-2	43.601.105.01-2	-	30.413.002.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES



STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0131	LAB SCANBODY	DAS_C_E_0131
DYNAMIC μSCANBODY (LAB/CLIN)	-	DYNAMIC μSCANBODY (LAB/CLIN)	-
	-		-

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



STANDARD DYNAMIC TIBASE®																	
GINGIVAL HEIGHT		α_s		α_c		GINGIVAL HEIGHT		α_s		α_c		GINGIVAL HEIGHT		α_s		α_c	
0,5 mm				mm				mm				mm					
R	31.324.132.01-2	45°	28°	-	-	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.314.132.01-2			-			-			-			-			-	

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α_s	α_s	α_s
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
-	-	-	-	-		-	-	33.345.856.01-2	3	25°
								33.445.856.01-2	4	
-	-							33.645.856.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27	ANALOG	LAB SCANBODY
41.316.081.01-2	-	43.618.201.01-2	18	40.316.005.08-2	43.601.105.01-2	-	30.414.003.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES



STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0132	LAB SCANBODY	DAS_C_E_0132
DYNAMIC μSCANBODY (LAB/CLIN)	-	DYNAMIC μSCANBODY (LAB/CLIN)	-
	-		-

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c
1 mm				mm				mm				mm			
R	31.320.135.01-2	45°	-	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.310.135.01-2			-			-		-			-			

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α_s	α_s	α_s
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
-	-	-	-	-		-	-	-	-	-
								-	-	
-	-							-	-	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER TORX T6	ANALOG	LAB SCANBODY
41.314.080.01-2	-	43.618.201.01-2	18	40.314.007.02-2	43.601.107.01-2	-	30.410.006.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES



STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0135	LAB SCANBODY	-
DYNAMIC μSCANBODY (LAB/CLIN)	-	DYNAMIC μSCANBODY (LAB/CLIN)	-
	-		-

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c
0,7 mm				1,5 mm				mm				3 mm			
R	31.320.136.01-2	45°	30°	31.320.136.02-2	25	-	-	-	-	31.320.136.04-2	20	-	-	-	-
NR	31.310.136.01-2			31.310.136.02-2			-			31.310.136.04-2					

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α_s	α_s	α_s
		CH=5mm	CH= 7mm	CH= 9mm
-	-	-	-	-
-	-			

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
52.410.128.01-2	10	50.310.136.01-2	43.621.415.01-2	34.610.136.01-2		-	-	33.360.754.01-2	3	25°
		50.310.136.04-2 IG=3mm						33.460.754.01-2	4	
52.412.128.01-2	12							33.660.754.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.25	ANALOG	LAB SCANBODY
41.316.071.01-2	-	43.618.201.01-2	18	40.316.004.03-2	43.601.104.01-2	-	30.410.006.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES



STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0136	LAB SCANBODY	DAS_C_E_0136
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0136	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0136
	DAS_IG_10_0136		DAS_C_IG_10_0136
	DAS_I_12_0136		DAS_C_I_12_0136
	DAS_IG_12_0136		DAS_C_IG_12_0136

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0137

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c
0,6 mm				mm				mm				mm			
R	31.324.137.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.314.137.01-2			-			-		-						

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
		CH=5mm	CH= 7mm	CH= 9mm
-	-	-	-	-
-	-			

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}
-	-	-	-	-		-	-	-	-	-
-	-							-	-	
-	-							-	-	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER TORX T6	ANALOG	LAB SCANBODY
41.320.044.01-2	-	43.618.201.01-2	18	40.320.007.04-2	43.601.107.01-2	-	30.414.008.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0137	LAB SCANBODY	DAS_C_E_0137
DYNAMIC μSCANBODY (LAB/CLIN)	-	DYNAMIC μSCANBODY (LAB/CLIN)	-
	-		-

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0149

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c
1,5 mm				mm				mm				mm			
R	31.323.149.01-2	45°	29°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.149.01-2			-				-				-			

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
		CH=5mm	CH= 7mm	CH= 9mm
-	-	-	-	-
-	-			

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}
52.410.132.01-2	10	50.310.161.01-2	43.621.410.01-2	34.610.161.01-2		-	-	33.320.704.01-2*	3	25°
-	-		43.624.410.01-2					33.420.704.01-2*	4	
52.412.132.01-2	12		43.630.410.01-2					33.620.704.01-2*	6	

*Only for R

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER -	ANALOG	LAB SCANBODY
41.316.079.01-2	-	43.618.201.01-2	18	40.316.014.01-2	-	-	30.413.002.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES



STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0149	LAB SCANBODY	DAS_C_E_0149
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0149	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0149
	DAS_I_12_0149		DAS_C_I_12_0149

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0150

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c
0,5 mm		45°	-	mm		-	-	mm		-	-	mm		-	-
R	31.323.150.01-2			-	-			-	-			-	-		
NR	-			-	-			-	-			-	-		

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
		CH=5mm	CH= 7mm	CH= 9mm
-	-	-	-	-
-	-			

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}
-	-	-	-	-		-	-	-	-	-
								-	-	
-	-								-	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.25	ANALOG	LAB SCANBODY
41.314.046.01-2	-	43.618.201.01-2	18	40.314.004.04-2	43.601.104.01-2	-	30.413.005.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0150	LAB SCANBODY	-
DYNAMIC μSCANBODY (LAB/CLIN)	-	DYNAMIC μSCANBODY (LAB/CLIN)	-
	-		-

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0151

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c
0,3 mm		45°	30°	mm		-	-	mm		-	-	mm		-	-
R	31.323.151.01-2			-	-			-	-			-	-		
-	-			-	-			-	-			-	-		

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
		CH=5mm	CH= 7mm	CH= 9mm
-	-	-	-	-
-	-			

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}
52.409.123.01-2	9	50.313.151.01-2	43.621.410.01-2	34.613.151.01-2		-	-	33.390.716.01-2	3	30°
			43.624.410.01-2					33.490.716.01-2	4	
			43.630.410.01-2					33.690.716.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER -	ANALOG	LAB SCANBODY
41.314.039.01-2	-	43.618.201.01-2	18	-	-	-	-
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	-	LAB SCANBODY	-
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_9_0151	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_9_0151

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0152

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
1 mm				mm				mm				mm			
R	31.320.152.01-2	45°	-	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.310.152.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α_s	α_s	α_s
		CH=5mm	CH= 7mm	CH= 9mm
-	-	-	-	-
-	-			

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
-	-	-	-	-		-	-	-	-	-
								-	-	
-	-							-	-	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER	ANALOG	LAB SCANBODY
41.318.077.02-2	-	43.618.201.01-2	18	-	-	-	30.410.006.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0152	LAB SCANBODY	-
DYNAMIC μSCANBODY (LAB/CLIN)	-	DYNAMIC μSCANBODY (LAB/CLIN)	-
	-		-

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

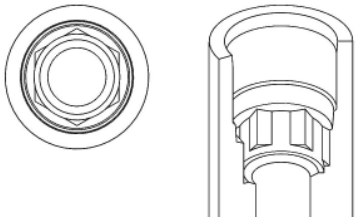

COMPATIBLE with 0159

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
1,5 mm				mm				mm				mm			
R	31.320.159.01-2	41°	17°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.310.159.01-2			-			-		-			-			

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α_s	α_s	α_s
		CH=5mm	CH= 7mm	CH= 9mm
-	-	-	-	-
-	-			

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
52.410.128.01-2	10	50.310.159.01-2	43.621.415.01-2	34.610.159.01-2		-	-	33.335.754.01-2*	3	25°
								33.435.754.01-2*	4	
-	-							33.635.754.01-2*	6	

*Only for R

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER UNIGRIP	ANALOG	LAB SCANBODY
41.314.067.02-2	-	43.618.201.01-2	18	40.314.008.02-2	43.601.108.01-2	22.610.159.01-2	30.410.006.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0159	LAB SCANBODY	DAS_C_E_0159
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0159	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0159

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

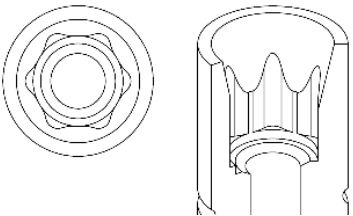

COMPATIBLE with 0160

STANDARD DYNAMIC TIBASE®																
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	
0,5 mm		45°	30°	mm	-	-	mm	-	-	mm	-	-	mm	-	-	
R	31.320.160.01-2			-			-			-			-			-
NR	31.310.160.01-2			-			-			-			-			-

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
		CH=5mm	CH= 7mm	CH= 9mm
-	-	-	-	-
-	-			

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL			SCANALOG
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT- CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}	SCANALOG	
52.410.131.01-2	10	50.310.160.01-2	43.621.415.01-2	34.610.160.01-2							
52.412.131.01-2	12										

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER TORX T6	LAB SCANBODY	
41.316.078.01-2	-	43.618.201.01-2	18	40.316.007.01-2	43.601.107.01-2	22.610.160.01-2	30.410.006.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES



STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0160	LAB SCANBODY	DAS_C_E_0160
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0160	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0160
	DAS_I_12_0160		DAS_C_I_12_0160
SCANALOG	DAS_SA_0160	SCANALOG	DAS_C_SA_0160

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0161

STANDARD DYNAMIC TIBASE®																
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	
1,5 mm		45°	25°	mm	-	-	mm	-	-	mm	-	-	mm	-	-	
R	31.320.161.01-2			-			-			-			-			-
NR	31.310.161.01-2			-			-			-			-			-

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
		CH=5mm	CH= 7mm	CH= 9mm
-	-	-	-	-
-	-			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL				
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT- CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}		
52.410.132.01-2	10	50.310.161.01-2	43.621.415.01-2	34.610.161.01-2			-	-	33.320.704.01-2*	3	25°
									33.420.704.01-2*	4	
52.412.132.01-2	12								33.620.704.01-2*	6	

*Only for R

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER -	LAB SCANBODY	
41.316.079.01-2	-	43.618.201.01-2	18	40.316.014.01-2	-	-	30.410.006.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES



STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0161	LAB SCANBODY	DAS_C_E_0161
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0161	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0161
	DAS_I_12_0161		DAS_C_I_12_0161

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0162

STANDARD DYNAMIC TIBASE®																	
GINGIVAL HEIGHT		α _s		α _c		GINGIVAL HEIGHT		α _s		α _c		GINGIVAL HEIGHT		α _s		α _c	
1,5 mm				mm				mm				mm					
R	31.324.162.01-2	45°	24°	-	-	-	-	-	-	-	-	-	-	-	-	-	-
NR	-			-			-			-			-				

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
		CH=5mm	CH= 7mm	CH= 9mm
-	-	-	-	-
-	-			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}
52.410.132.01-2	10	50.310.161.01-2	43.621.415.01-2	34.610.161.01-2	-	-	33.320.704.01-2*	3	25°
							33.420.704.01-2*	4	
52.412.132.01-2	12						33.620.704.01-2*	6	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER	ANALOG	LAB SCANBODY
41.316.079.01-2	-	43.618.201.01-2	18	40.316.014.01-2	-	-	30.414.003.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

COMPATIBLE with 0163

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c
0,5 mm				mm			mm			mm			mm		
R	31.323.163.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	-			-			-			-			-		

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
		CH=5mm	CH= 7mm	CH= 9mm
-	-	-	-	-
-	-			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}
52.408.112.01-2	8	50.313.163.01-2	43.620.411.01-2	34.613.163.01-2	-	-	33.390.716.01-2	3	30°
							33.490.716.01-2	4	
							33.690.716.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER	ANALOG	LAB SCANBODY
41.314.039.01-2	-	43.618.201.01-2	18	40.314.014.01-2	-	-	30.413.005.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

COMPATIBLE with 0164

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c
1 mm				mm			mm			mm			mm		
R	31.320.164.01-2	45°	21°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.310.164.01-2			-			-			-			-		

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
		CH=5mm	CH= 7mm	CH= 9mm
-	-	-	-	-
-	-			

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}
-	-	-	-	-		-	-	33.345.804.01-2*	3	25°
								33.445.804.01-2*	4	
-	-							33.645.804.01-2*	6	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER	ANALOG	LAB SCANBODY
41.312.078.01-2	-	43.618.201.01-2	18	-	-	-	30.413.006.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES



STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0164	LAB SCANBODY	DAS_C_E_0164
DYNAMIC μSCANBODY (LAB/CLIN)	-	DYNAMIC μSCANBODY (LAB/CLIN)	-
	-		-

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0165

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c	GINGIVAL HEIGHT	α _s	α _c
1 mm				mm			mm			mm			mm		
R	31.323.165.01-2	45°	25°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.165.01-2			-			-			-			-		

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
		CH=5mm	CH= 7mm	CH= 9mm
-	-	-	-	-
-	-			

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}
52.410.132.01-2	10	50.313.165.01-2	43.621.415.01-2	34.613.165.01-2		-	-	33.345.804.01-2*	3	30°
								33.445.804.01-2*	4	
52.412.132.01-2	12							33.645.804.01-2*	6	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.20	ANALOG	LAB SCANBODY
41.314.076.01-2	-	43.618.201.01-2	18	-	43.601.103.02-2	-	30.413.002.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES



STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0165	LAB SCANBODY	DAS_C_E_0165
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0165	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0165
	DAS_I_12_0165		DAS_C_I_12_0165

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0166

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c
0,9 mm				mm				mm				mm			
R	31.320.166.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.310.166.01-2			-			-		-						

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
		CH=5mm	CH= 7mm	CH= 9mm
-	-	-	-	-
-	-			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}
52.410.128.01-2	10	50.310.166.03-2 IG=3mm	43.621.415.01-2	34.610.166.01-2	-	-	-	-	-
							-	-	
-	-						-	-	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.25	ANALOG	LAB SCANBODY
41.314.084.01-2	-	43.618.201.01-2	18	40.314.004.02-2	43.601.104.01-2	-	30.410.006.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

COMPATIBLE with 0167

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c
0,9 mm				mm				mm				mm			
R	31.322.167.01-2	43°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.312.167.01-2			-			-		-						

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
		CH=5mm	CH= 7mm	CH= 9mm
-	-	-	-	-
-	-			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}
52.410.117.01-2	10	50.313.167.03-2 (IG= 3mm)	43.620.411.01-2	34.613.167.01-2	-	-	33.330.734.01-2	3	20°
			43.621.410.01-2				33.430.734.01-2	4	
52.412.117.01-2	12		43.624.410.01-2				33.630.734.01-2	6	



DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.25	ANALOG	LAB SCANBODY
41.316.084.02-2	-	43.618.201.01-2	18	-	-	-	30.412.001.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0167	LAB SCANBODY	DAS_C_E_0167
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_IG_10_0167	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_IG_10_0167
	DAS_IG_12_0167		DAS_C_IG_12_0167

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height
IG = Adaptor 3mm
α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0168

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c
0,3 mm				mm				mm				mm			
R	31.323.168.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	-			-			-		-						

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
		CH=5mm	CH= 7mm	CH= 9mm
-	-	-	-	-
-	-			

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}
-	-	-	-	-		-	-	-	-	-
-	-							-	-	
-	-							-	-	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27	ANALOG	LAB SCANBODY
41.314.039.01-2	-	43.618.201.01-2	18	40.314.004.03-2	43.601.104.01-2	-	30.413.005.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

COMPATIBLE with 0169

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c
0,6 mm				1,5 mm				mm				3 mm			
R	31.322.169.01-2	45°	29°	31.322.169.02-2	25	-	-	-	-	31.322.169.04-2	20	-	-	-	-
NR	31.312.169.01-2			31.312.169.02-2			-						31.312.169.04-2		

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
		CH=5mm	CH= 7mm	CH= 9mm
-	-	-	-	-
-	-			

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}
52.410.117.01-2	10	50.312.169.01-2 50.312.169.04-2 IG=3mm	43.621.410.01-2	34.612.169.01-2		-	-	33.330.734.01-2	3	25°
-	-		43.624.410.01-2					33.430.734.01-2	4	
52.412.117.01-2	12		43.630.410.01-2					33.630.734.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER -	ANALOG	LAB SCANBODY
41.317.070.01-2	-	43.618.201.01-2	18	-	-	-	30.412.001.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				



LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0169	LAB SCANBODY	DAS_C_E_0169
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0169	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0169
	DAS_IG_10_0169		DAS_C_IG_10_0169
	DAS_I_12_0169		DAS_C_I_12_0169
	DAS_IG_12_0169		DAS_C_IG_12_0169

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height
IG = Adaptor (3mm)

α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0170

STANDARD DYNAMIC TIBASE®													
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT	
0,3 mm				mm				mm				mm	
R	31.322.170.01-2	38°	-	-	-	-	-	-	-	-	-	-	-
NR	31.312.170.01-2			-				-				-	

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α_s	α_c	α_s
0,3 mm		CH=5mm	CH= 7mm	CH= 9mm
R	31.322.170.21-2	30°	20°	15°
NR	31.312.170.21-2			

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
-	-	-	-	-		-	-	33.390.754.01-2	3	25°
								33.490.754.01-2	4	
-	-							33.690.754.01-2	6	


DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.20	ANALOG	LAB SCANBODY
41.316.079.02-2	-	43.618.201.01-2	18	-	-	-	30.410.006.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0170	LAB SCANBODY	-
DYNAMIC μSCANBODY (LAB/CLIN)	-	DYNAMIC μSCANBODY (LAB/CLIN)	-
	-		-

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height
IG= Adaptor (3mm)
 α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

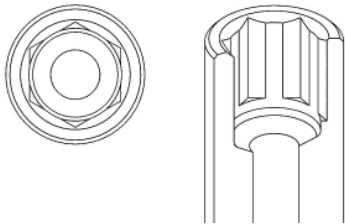

COMPATIBLE with 0171

STANDARD DYNAMIC TIBASE®													
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT	
0,3 mm				mm				mm				mm	
R	31.323.171.01-2	35°	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.171.01-2			-				-				-	

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α_s	α_c	α_s
		CH=5mm	CH= 7mm	CH= 9mm
-	-	-	-	-
-	-			

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
-	-	-	-	-		-	-	33.390.754.01-2	3	25°
								33.490.754.01-2	4	
-	-							33.690.754.01-2	6	


DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.20	ANALOG	LAB SCANBODY
41.316.079.02-2	-	43.618.201.01-2	18	-	-	-	30.412.001.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0171	LAB SCANBODY	-
DYNAMIC μSCANBODY (LAB/CLIN)	-	DYNAMIC μSCANBODY (LAB/CLIN)	-
	-		-

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height
 α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

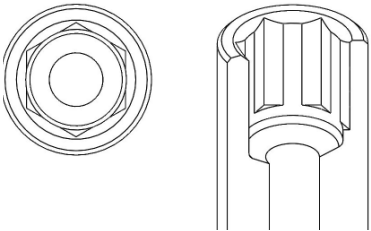

COMPATIBLE with 0178

STANDARD DYNAMIC TIBASE®													
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT	
1,5 mm				mm				mm				mm	
R	31.320.178.01-2	45°	-	-	-	-	-	-	-	-	-	-	-
NR	31.310.178.01-2		-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α_s	α_s	α_s
		CH=5mm	CH= 7mm	CH= 9mm
-	-	-	-	-
-	-	-	-	-

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
-	-	-	-	-	-	-	-	-	-	-
-	-							-	-	
-	-							-	-	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER -	ANALOG	LAB SCANBODY
41.316.080.01-2	-	43.618.201.01-2	18	-	-	-	30.410.006.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES



STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0178	LAB SCANBODY	-
DYNAMIC μSCANBODY (LAB/CLIN)	-	DYNAMIC μSCANBODY (LAB/CLIN)	-
	-		-

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0181

STANDARD DYNAMIC TIBASE®													
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT	
mm				mm				mm				mm	
R	-	-	-	-	-	-	-	-	-	-	-	-	-
NR	-			-	-			-	-			-	-

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α_s	α_s	α_s
0,4 mm		CH=5mm	CH= 7mm	CH= 9mm
R	31.322.181.21-2	30°	25°	10°
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		SCANALOG
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
52.408.112.01-2	8	50.312.181.01-2	43.620.411.01-2	-	-	-	-	33.360.756.01-2	3	30°
-	-							33.460.756.01-2	4	
-	-							33.660.756.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER -	ANALOG	LAB SCANBODY
41.318.043.01-2	-	43.618.201.01-2	18	-	-	-	-
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES



STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0181	LAB SCANBODY	-
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_8_0181	DYNAMIC μSCANBODY (LAB/CLIN)	-
SCANALOG	DAS_SA_0101	SCANALOG	-

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



STANDARD DYNAMIC TIBASE®														
GINGIVAL HEIGHT 1,2 mm			GINGIVAL HEIGHT 2,5 mm			GINGIVAL HEIGHT 3,5 mm			GINGIVAL HEIGHT mm			GINGIVAL HEIGHT mm		
α _s	α _c		α _s	α _c		α _s	α _c		α _s	α _c		α _s	α _c	
R	31.323.186.01-2	40°	30°	31.323.186.02-2	20°	18°	31.323.186.03-2	15°	-	°	°	-	°	°
NR	31.313.186.01-2			31.313.186.02-2			31.313.186.03-2		-	°	°	-	°	°

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
		CH=5mm	CH= 7mm	CH= 9mm
-	-	-	-	-
-	-	-	-	-

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT- CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}
54.408.101.01-2	8	50.313.186.04-2 (IG=3mm)	43.621.410.01-2	34.613.186.01-2		-	-	33.330.734.01-2	3	25
54.410.101.01-2	10		43.624.410.01-2					33.430.734.01-2	4	
54.412.101.01-2	12		43.630.410.01-2					33.630.734.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER -	ANALOG	LAB SCANBODY
41.316.084.02-2	-	43.618.201.01-2	18	-	-	-	30.413.002.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				


LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0186	LAB SCANBODY	DAS_C_E_0186
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_IG_8_0186	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_IG_8_0186
	DAS_IG_10_0186		DAS_C_IG_10_0186
	DAS_IG_12_0186		DAS_C_IG_12_0186

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height
IG = Adaptor (3mm)

α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

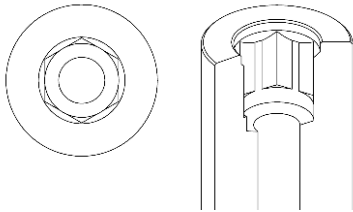

STANDARD DYNAMIC TIBASE®														
GINGIVAL HEIGHT 0,3 mm			GINGIVAL HEIGHT 0,5 mm			GINGIVAL HEIGHT 1 mm			GINGIVAL HEIGHT mm			GINGIVAL HEIGHT mm		
α _s	α _c		α _s	α _c		α _s	α _c		α _s	α _c		α _s	α _c	
R	31.322.009.01-2	45°	25°	31.322.009.02-2	25°	25°	31.322.009.03-2	25°	-	-	-	-	-	-
NR	31.312.009.01-2			31.312.009.02-2			31.312.009.03-2		-	-	-	-	-	-

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _s	α _s
		CH=5mm	CH= 7mm	CH= 9mm
-	-	-	-	-
-	-	-	-	-

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT- CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}
52.410.114.01-2	10	50.312.187.01-2	43.621.410.01-2	34.612.187.01-2		-	-	33.390.716.01-2	3	25°
			43.624.410.01-2					33.490.716.01-2	4	
52.412.114.01-2	12		43.630.410.01-2					33.690.716.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER -	ANALOG	LAB SCANBODY
41.316.059.01-2	-	43.618.201.01-2	18	-	-	-	30.412.001.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				


LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0187	LAB SCANBODY	DAS_C_E_0187
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0187	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0187
	DAS_I_12_0187		DAS_C_I_12_0187

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

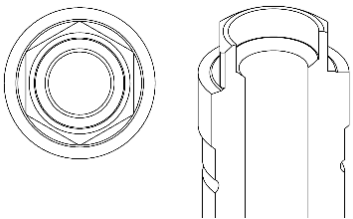

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c
1,8 mm				mm				mm				mm			
R	31.320.190.01-2	45°	-	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.310.190.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α_s	α_s	α_s
		CH=5mm	CH= 7mm	CH= 9mm
-	-	-	-	-
-	-			

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
-	-	-	-	-	-	-	-	-	-	-
-	-							-	-	
-	-							-	-	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER	ANALOG	LAB SCANBODY
41.316.084.02-2	-	43.618.201.01-2	18	-	-	-	30.410.006.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0190	LAB SCANBODY	-
DYNAMIC μSCANBODY (LAB/CLIN)	-	DYNAMIC μSCANBODY (LAB/CLIN)	-
	-		-
	-		-

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

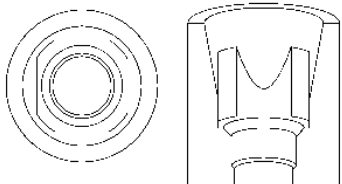

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
0,8 mm				mm				mm				mm			
R	31.322.191.01-2	45°	-	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.312.191.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α_s	α_s	α_s
		CH=5mm	CH= 7mm	CH= 9mm
-	-	-	-	-
-	-			

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
-	-	-	-	-	-	-	-	-	-	-
-	-							-	-	
-	-							-	-	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER	ANALOG	LAB SCANBODY
41.316.084.02-2	-	43.618.201.01-2	18	-	-	-	30.412.001.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0191	LAB SCANBODY	-
DYNAMIC μSCANBODY (LAB/CLIN)	-	DYNAMIC μSCANBODY (LAB/CLIN)	-
	-		-
	-		-

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

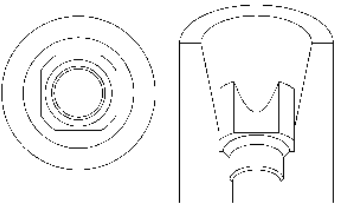

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
0,3 mm				mm				mm				mm			
R	31.323.192.01-2	45°	-	-	-	-	-	-	-	-	-	-	-	-	-
-	-			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α_s	α_s	α_s
		CH=5mm	CH= 7mm	CH= 9mm
-	-	-	-	-
-	-			

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
-	-	-	-	-	-	-	-	-	-	-
-	-							-	-	
-	-							-	-	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER	ANALOG	LAB SCANBODY
41.316.048.01-2	-	43.618.201.01-2	18	-	-	-	30.413.005.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
0,3 mm				mm				mm				mm			
R	31.323.193.01-2	45°	-	-	-	-	-	-	-	-	-	-	-	-	-
-	-			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α_s	α_s	α_s
		CH=5mm	CH= 7mm	CH= 9mm
-	-	-	-	-
-	-			

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
-	-	-	-	-	-	-	-	-	-	-
-	-							-	-	
-	-							-	-	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER	ANALOG	LAB SCANBODY
41.318.051.02-2	-	43.618.201.01-2	18	-	-	-	30.413.005.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

STANDARD DYNAMIC TIBASE®														
GINGIVAL HEIGHT 1,2 mm			GINGIVAL HEIGHT 2 mm			GINGIVAL HEIGHT mm			GINGIVAL HEIGHT mm			GINGIVAL HEIGHT mm		
R	31.320.196.01-2	40°	-	31.320.196.02-2	25°	-	-	-	-	°	°	-	°	°
NR	31.310.196.01-2			31.310.196.02-2		-	-	-	-	°	°	-	°	°

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _c	α _s
		CH=5mm	CH= 7mm	CH= 9mm
-	-	-	-	-
-	-	-	-	-

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT- CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}
-	-	-	-	-		-	-	-	-	-
								-	-	
-	-							-	-	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER -	ANALOG	LAB SCANBODY
41.316.086.01-2	-	43.618.201.01-2	18	-	-	-	30.410.006.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES



STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0196	LAB SCANBODY	-
DYNAMIC μSCANBODY (LAB/CLIN)	-	DYNAMIC μSCANBODY (LAB/CLIN)	-
	-		-

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



STANDARD DYNAMIC TIBASE®														
GINGIVAL HEIGHT 1,2 mm			GINGIVAL HEIGHT 2 mm			GINGIVAL HEIGHT mm			GINGIVAL HEIGHT mm			GINGIVAL HEIGHT mm		
R	31.322.197.01-2	35°	-	31.322.197.02-2	20°	-	-	-	-	°	°	-	°	°
NR	31.312.197.01-2			31.312.197.02-2		-	-	-	-	°	°	-	°	°

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α _s	α _c	α _s
		CH=5mm	CH= 7mm	CH= 9mm
-	-	-	-	-
-	-	-	-	-

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT- CHROME	α _{dp}	DYNAMIC MILLING TOOL	SHANK	α _{di}
-	-	-	-	-		-	-	-	-	-
								-	-	
-	-							-	-	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER -	ANALOG	LAB SCANBODY
41.316.086.01-2	-	43.618.201.01-2	18	-	-	-	30.412.001.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES



STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0197	LAB SCANBODY	-
DYNAMIC μSCANBODY (LAB/CLIN)	-	DYNAMIC μSCANBODY (LAB/CLIN)	-
	-		-

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
α_c = Captive maximum angulation
α_{di} = Direct to implant maximum angulation
α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c
1,2 mm				mm				mm				mm			
R	31.324.198.01-2	40°	-	-	-	-	-	-	-	°	°	-	°	°	
NR	31.314.198.01-2			-	-	-	-	-	-	°	°	-	°	°	

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α_s	α_s	α_s
		CH=5mm	CH= 7mm	CH= 9mm
-	-	-	-	-
-	-			

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
-	-	-	-	-	-	-	-	-	-	-
-	-							-	-	
-	-							-	-	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER	ANALOG	LAB SCANBODY
41.316.086.01-2	-	43.618.201.01-2	18	-	-	-	30.414.003.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0198	LAB SCANBODY	-
DYNAMIC μSCANBODY (LAB/CLIN)	-	DYNAMIC μSCANBODY (LAB/CLIN)	-
	-		-

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

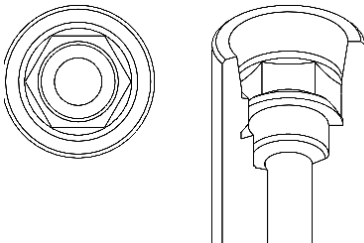

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
0,3 mm				mm				mm				mm			
R	31.322.205.01-2	45°	-	-	°	°	-	°	°	-	°	°	-	°	°
NR	-			-	°	°	-	°	°	-	°	°	-	°	°

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α_s	α_s	α_s
		CH=5mm	CH= 7mm	CH= 9mm
-	-	-	-	-
-	-			

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
-	-	-	-	-	-	-	-	-	-	-
-	-							-	-	
-	-							-	-	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER	ANALOG	LAB SCANBODY
41.317.040.01-2	-	43.618.201.01-2	18	-	Hex. 1.27	-	30.412.001.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0205	LAB SCANBODY	-
DYNAMIC μSCANBODY (LAB/CLIN)	-	DYNAMIC μSCANBODY (LAB/CLIN)	-
	-		-

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

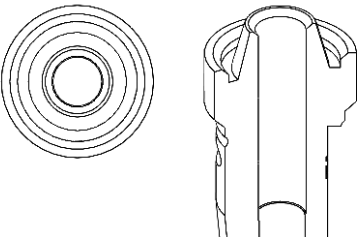

COMPATIBLE with 0207

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c
1,5 mm				mm				mm				mm			
R	31.320.207.01-2	40°	-	-	-	-	-	-	-	°	°	-	°	°	
NR	31.310.207.01-2			-	-	-	-	-	-	°	°	-	°	°	

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α_s	α_s	α_s
		CH=5mm	CH= 7mm	CH= 9mm
-	-	-	-	-
-	-			

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
-	-	-	-	-		-	-	-	-	-
								-	-	
-	-							-	-	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER	ANALOG	LAB SCANBODY
41.316.066.01-2	-	43.618.201.01-2	18	-	-	-	30.410.006.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0207	LAB SCANBODY	-
DYNAMIC μSCANBODY (LAB/CLIN)	-	DYNAMIC μSCANBODY (LAB/CLIN)	-
	-		-

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

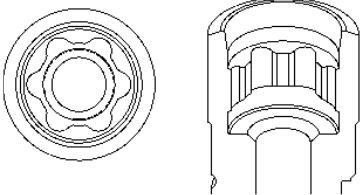

COMPATIBLE with 0208

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c	GINGIVAL HEIGHT		α _s	α _c
1,5 mm				mm				mm				mm			
R	31.324.208.01-2	45°	-	-	°	°	-	°	°	-	°	°	-	°	°
NR	31.314.208.01-2			-	°	°	-	°	°	-	°	°	-	°	°

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α_s	α_s	α_s
		CH=5mm	CH= 7mm	CH= 9mm
-	-	-	-	-
-	-			

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
-	-	-	-	-		-	-	-	-	-
								-	-	
-	-							-	-	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER	ANALOG	LAB SCANBODY
41.316.066.01-2	-	43.618.201.01-2	18	-	Hex. 1.27	-	30.414.003.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0208	LAB SCANBODY	-
DYNAMIC μSCANBODY (LAB/CLIN)	-	DYNAMIC μSCANBODY (LAB/CLIN)	-
	-		-

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height



α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

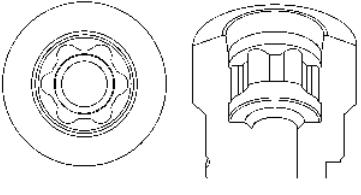

DYNAMIC SCREWS TECHNICAL SPECIFICATIONS

REFERENCE	METRIC	TORQUE	TOTAL LENGTH	THREAD LENGTH	A LENGTH	B LENGTH	C LENGTH	HEAD DIAMETER	SEAT	ANGLE	THREAD ENTRY	CONNECTION
41.312.078.01-2	1,2	15 N·cm	7,8	2,65	6	6,55	1,25	2,3	conical	45°	45° Chamfer	HEXALOBULAR 1,70
41.314.039.01-2	1,4	15 N·cm	3,9	1,8	2,1	-	1,8	2,4	straight	-	45° Chamfer	
41.314.040.01-2	1,4	15 N·cm	4	1,85	2	2,78	1,22	2,3	conical	30°	45° Chamfer	
41.314.040.02-2	1,4	15 N·cm	4	1,7	2,25	2,7	1,3	2,3	conical	45°	45° Chamfer	
41.314.043.01-2	1,4	15 N·cm	4,3	1,8	2,03	2,9	1,4	2,3	conical	35°	45° Chamfer	
41.314.045.01-2	1,4	15 N·cm	4,5	2,3	2,5	3,28	1,22	2,3	conical	30°	45° Chamfer	
41.314.046.01-2	1,4	15 N·cm	4,6	2,5	4,6	3,17	1,43	2,3	conical	35°	45° Chamfer	
41.314.052.01-2	1,4	15 N·cm	5,2	2,9	3,4	-	1,8	2,3	straight	-	45° Chamfer	
41.314.064.01-2	1,4	15 N·cm	6,4	2,2	4,21	5,15	1,25	2,3	conical	25°	45° Chamfer	
41.314.064.02-2	1,4	15 N·cm	6,4	2,2	4,65	-	1,75	2,3	straight	-	45° Chamfer	
41.314.067.01-2	1,4	15 N·cm	6,7	2,31	5	5,45	1,25	2,3	conical	45°	45° Chamfer	
41.314.067.02-2	1,4	15 N·cm	6,7	2,5	4,71	5,5	1,2	2,3	conical	35°	45° Chamfer	
41.314.070.01-2	1,4	15 N·cm	7	2,3	5,39	5,65	1,61	2,3	conical	60°	45° Chamfer	
41.314.074.01-2	1,4	15 N·cm	7,4	3,55	5	5,99	1,41	2,3	conical	25°	45° Chamfer	
41.314.076.01-2	1,4	15 N·cm	7,6	2,4	5,9	6,35	1,25	2,3	conical	45°	45° Chamfer	
41.314.080.01-2	1,4	15 N·cm	8	2,1	4,96	6,8	1,2	2,3	conical	15°	45° Chamfer	
41.314.084.01-2	1,4	15 N·cm	8,4	2,5	5,92	6,85	1,55	2,3	conical	35°	45° Chamfer	
41.314.105.01-2	1,4	15 N·cm	10,5	2,31	5	5,45	5,05	2,3	conical	45°	45° Chamfer	
41.316.044.01-2	1,6	20 N·cm	4,4	2,5	2,9	-	1,5	2,3	straight	-	Semi-sphere	
41.316.048.01-2	1,6	20 N·cm	4,8	2,4	2,93	1,87	1,3	2,3	conical	45	45° Chamfer	
41.316.055.01-2	1,6	20 N·cm	5,5	2,4	2,85	4,2	1,3	2,3	conical	23°	45° Chamfer	
41.316.059.01-2	1,6	20 N·cm	5,9	3	4,4	-	1,5	2,3	straight	-	Semi-sphere	
41.316.066.01-2	1,6	20 N·cm	6,6	1,9	4,7	5,2	1,9	2,3	conical	45°	45° Chamfer	
41.316.071.01-2	1,6	20 N·cm	7,1	2,8	5,2	5,53	1,57	2,3	conical	60°	45° Chamfer	
41.316.072.01-2	1,6	20 N·cm	7,2	3,5	5,2	5,85	1,35	2,3	conical	30°	45° Chamfer	
41.316.073.01-2	1,6	20 N·cm	7,3	2,2	4,87	5,56	1,74	2,3	conical	35°	45° Chamfer	

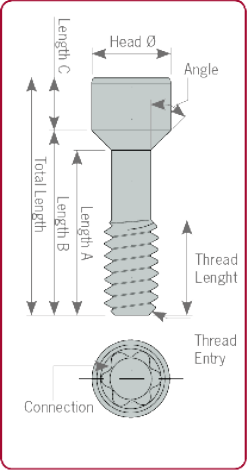
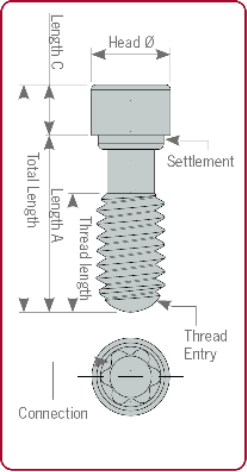


REFERENCE	METRIC	TORQUE	TOTAL LENGTH	THREAD LENGTH	A LENGTH	B LENGTH	C LENGTH	HEAD DIAMETER	SEAT	ANGLE	THREAD ENTRY	CONNECTION
41.316.074.01-2	1,6	20 N·cm	7,4	2,7	5,5	6	1,4	2,3	conical	45°	45° Chamfer	HEXALOBULAR 1,70
41.316.076.01-2	1,6	20 N·cm	7,6	3,6	6,1	-	1,5	2,3	straight	-	Semi-sphere	
41.316.078.01-2	1,6	20 N·cm	7,8	2	5,36	7,03	0,81	2,3	conical	15°	45° Chamfer	
41.316.079.01-2	1,6	20 N·cm	7,9	2,30	5,42	6,60	1,3	2,3	conical	20°	45° Chamfer	
41.316.079.02-2	1,6	20 N·cm	7,9	3,9	6,3	-	1,6	2,3	straight	-	45° Chamfer	
41.316.080.01-2	1,6	20 N·cm	8	3,14	6,3	6,51	1,49	2,3	conical	60°	45° Chamfer	
41.316.081.01-2	1,6	20 N·cm	8,1	3	6,35	6,72	1,38	2,3	conical	45°	45° Chamfer	
41.316.084.01-2	1,6	20 N·cm	8,4	3,5	6,8	-	1,6	2,3	straight	-	Semi-sphere	
41.316.084.02-2	1,6	20 N·cm	8,4	2,7	5,85	6,85	1,55	2,3	conical	30°	45° Chamfer	
41.316.086.01-2	1,6	20 N·cm	8,6	3	7,2	-	1,4	2,3	straight	-	45° Chamfer	
41.316.094.01-2	1,6	20 N·cm	9,4	2,9	7,65	8	1,4	2,3	conical	45°	45° Chamfer	
41.316.094.02-2	1,6	20 N·cm	9,4	2,9	7,9	-	1,5	2,3	straight	-	45° Chamfer	
41.316.108.01-2	1,6	20 N·cm	10,8	2	5,36	7,03	0,81	2,3	conical	15°	45° Chamfer	
41.316.115.01-2	1,6	20 N·cm	11,5	3,5	5,2	5,85	6,3	2,3	conical	30°	45° Chamfer	
41.316.118.01-2	1,6	20 N·cm	11,8	3,6	6,1	-	5,7	2,3	straight	-	Semi-sphere	
41.316.124.01-2	1,6	20 N·cm	12,4	2,2	4,74	5,56	5,24	2,3	conical	35°	45° Chamfer	
41.316.132.01-2	1,6	20 N·cm	13,2	2,9	7,62	8	5,2	2,3	conical	45°	45° Chamfer	
41.317.040.01-2	N1-72	25 N·cm	4	2,1	2,5	-	1,5	2,3	sraight	-	45° Chamfer	
41.317.065.01-2	N1-72	25 N·cm	6,5	2,4	4,7	5,18	1,33	2,3	conical	45°	45° Chamfer	
41.317.070.01-2	N1-72	25 N·cm	7	2,2	4,96	5,8	1,2	2,3	conical	30°	45° Chamfer	
41.317.071.01-2	N1-72	25 N·cm	7,1	2,6	5,56	5,65	1,45	2,3	conical	70°	45° Chamfer	
41.317.071.02-2	N1-72	25 N·cm	7,1	2,6	5,6	-	1,5	2,3	straight	-	45° Chamfer	
41.317.073.01-2	N1-72	25 N·cm	7,3	2,5	5,5	5,77	1,53	2,3	conical	60°	45° Chamfer	
41.317.106.01-2	N1-72	25 N·cm	10,6	2,6	5,54	5,65	4,95	2,3	conical	70°	Semi-sphere	
41.318.035.01-2	1,8	25 N·cm	3,5	1,9	1,93	2,2	1,4	2,3	conical	60°	45° Chamfer	
41.318.043.01-2	1,8	25 N·cm	4,3	2	2,52	2,7	1,6	2,3	conical	55°	45° Chamfer	
41.318.044.01-2	1,8	25 N·cm	4,4	2,75	3	-	1,4	2,3	straight	-	Semi-sphere	
41.318.045.01-2	1,8	25 N·cm	4,5	2,3	2,81	2,9	1,6	2,3	conical	70°	45° Chamfer	



DYNAMIC SCREWS TECHNICAL SPECIFICATIONS

REFERENCE	METRIC	TORQUE	TOTAL LENGTH	THREAD LENGTH	A LENGTH	B LENGTH	C LENGTH	HEAD DIAMETER	SEAT	ANGLE	THREAD ENTRY	CONNECTION
41.318.048.01-2	1,8	25 N-cm	4,8	2,8	3,22	3,65	1,15	2,3	conical	30°	Semi-sphere	Hexalobular 1,70
41.318.051.01-2	1,8	25 N-cm	5,1	2,7	3,55	3,7	1,4	2,3	conical	60°	45° Chamfer	
41.318.051.02-2	1,8	25 N-cm	5,1	2,7	3,55	3,7	1,4	2,3	conical	45°	45° Chamfer	
41.318.064.01-2	1,8	25 N-cm	6,4	3,45	4,73	5,1	1,3	2,3	conical	35°	45° Chamfer	
41.318.065.01-2	1,8	25 N-cm	6,5	2,8	5	-	1,5	2,3	straight	-	Semi-sphere	
41.318.067.01-2	1,8	25 N-cm	6,7	2,35	5	5,4	1,3	2,3	conical	45°	45° Chamfer	
41.318.068.01-2	1,8	25 N-cm	6,8	4	5,25	5,4	1,4	2,3	conical	60°	45° Chamfer	
41.318.071.01-2	1,8	25 N-cm	7,1	2,6	5,56	5,65	1,45	2,3	conical	70°	45° Chamfer	
41.318.074.01-2	1,8	25 N-cm	7,4	3,8	5,8	6,03	1,6	2,3	conical	50°	45° Chamfer	
41.318.075.01-2	1,8	25 N-cm	7,5	3,3	6,1	-	1,4	2,3	straight	-	Semi-sphere	
41.318.076.01-2	1,8	25 N-cm	7,6	2,52	5,8	6,2	1,4	2,3	conical	45°	45° Chamfer	
41.318.077.01-2	1,8	25 N-cm	7,7	2,5	5,81	1,89	1,2	2,3	conical	30°	45° Chamfer	
41.318.077.02-2	1,8	25 N-cm	7,7	2	6,09	6,35	1,35	2,3	conical	60°	45° Chamfer	
41.318.080.01-2	1,8	25 N-cm	8	4	6,5	-	1,5	2,3	straight	-	45° Chamfer	
41.318.083.01-2	1,8	25 N-cm	8,3	4,25	6,79	6,95	1,35	2,3	conical	60°	45° Chamfer	
41.320.038.01-2	2	25 N-cm	3,81	1,6	3,25	2,35	1,39	2,35	conical	70°	20° Chamfer	
41.320.044.01-2	2	25 N-cm	4,4	2,45	2,45	3,1	1,3	2,3	conical	45°	45° Chamfer	
41.320.047.01-2	2	25 N-cm	4,7	3	3,3	-	1,4	2,3	straight	-	Semi-sphere	
41.320.048.01-2	2	25 N-cm	4,8	2,7	3,3	3,4	1,4	2,3	conical	60°	45° Chamfer	
41.320.050.01-2	2	25 N-cm	5	2,8	3,39	3,6	1,4	2,3	conical	30°	Semi-sphere	
41.320.051.01-2	2	25 N-cm	5,1	3,1	3,6	-	1,5	2,3	straight	-	Semi-sphere	
41.320.060.01-2	2	25 N-cm	6	2,7	4,5	-	1,5	2,3	straight	-	Semi-sphere	
41.320.065.01-2	2	25 N-cm	6,5	2,7	5	-	1,5	2,3	straight	-	45° Chamfer	
41.320.067.01-2	2	25 N-cm	6,7	2,3	3,65	5,68	1,02	2,58	conical	15°	45° Chamfer	
41.320.068.01-2	2	25 N-cm	6,8	4,4	5,3	5,4	1,4	2,3	conical	60°	45° Chamfer	

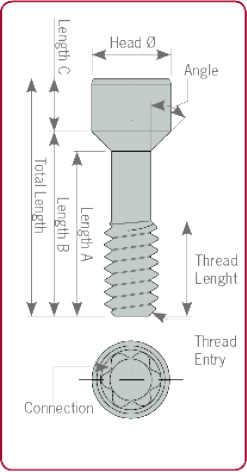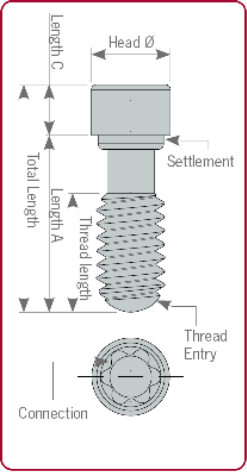

REFERENCE	METRIC	TORQUE	TOTAL LENGTH	THREAD LENGTH	A LENGTH	B LENGTH	C LENGTH	HEAD DIAMETER	SEAT	ANGLE	THREAD ENTRY	CONNECTION
41.320.070.01-2	2	25 N-cm	7	3	5,6	-	1,4	2,3	straight	-	Semi-sphere	Hexalobular 1,70
41.320.074.01-2	2	25 N-cm	7,4	3,3	6	-	1,4	2,3	straight	-	Semi-sphere	
41.320.075.01-2	2	25 N-cm	7,5	2,75	5,93	6,18	1,32	2,3	conical	35°	45° Chamfer	
41.320.079.01-2	2	25 N-cm	7,9	3,3	6,33	6,5	1,4	2,3	conical	45°	45° Chamfer	
41.320.082.01-2	2	25 N-cm	8,2	4,7	6,7	-	1,5	2,4	straight	-	Semi-sphere	
41.320.090.01-2	2	25 N-cm	9	4	7,5	-	1,5	2,3	straight	-	Semi-sphere	
41.320.094.01-2	2	25 N-cm	9,4	3	7,85	8	1,4	2,3	conical	45°	45° Chamfer	
41.320.094.02-2	0	25 N-cm	9,4	3	7,9	-	1,5	2,3	straight	-	45° Chamfer	
41.320.117.01-2	2	25 N-cm	11,7	2,75	5,9	6,18	5,52	2,3	conical	35°	Semi-sphere	
41.320.125.01-2	2	25 N-cm	12,5	3,3	6,33	6,5	6	2,3	conical	45°	45° Chamfer	
41.320.137.01-2	2	25 N-cm	13,7	4	12,2	-	1,5	2,3	straight	-	Semi-sphere	
41.325.054.01-2	2,5	25 N-cm	5,4	3,8	4,1	-	1,3	2,85	straight	-	Semi-sphere	
41.325.067.01-2	2,5	25 N-cm	6,7	4,6	5,1	-	1,6	2,85	straight	-	Semi-sphere	

DYNAMIC SCREWDRIVER & DYNAMIC SCREWS

Dynamic Screwdrivers

Screwdriver with hexalobular head, exclusively to the 3.0 Dynamic Abutment® system.

Lengths: 18, 24, 32mm.



Dynamic Screws are used with the Dynamic TiBase® or milled structures with an angled screw channel. Made of Titanium grade V.





High Dynamic Screw

Dynamic Screw

STRAIGHT SCREWS TECHNICAL SPECIFICATIONS

REFERENCE	METRIC	TORQUE	TOTAL LENGTH	THREAD LENGTH	A LENGTH	B LENGTH	C LENGTH	HEAD DIAMETER	SEAT	ANGLE	THREAD ENTRY	CONNECTION
40.312.003.01-2	1,2	15 N-cm	7,85	2,7	6,19	6,55	1,3	1,9	conical	45°	45° Chamfer	Hex. 1,20
40.314.003.01-2	1,4	15 N-cm	3,9	1,91	2,1	-	1,8	2,4	straight	-	45° Chamfer	Hex. 1,20
40.314.003.02-2	1,4	15 N-cm	4	2	2,2	-	1,8	2,3	straight	-	45° Chamfer	Hex. 1,20
40.314.003.03-2	1,4	15 N-cm	7,6	2,4	6,05	6,3	1,3	1,9	conical	45°	45° Chamfer	Hex. 1,20
40.314.003.04-2	1,4	15 N-cm	7,5	2,5	5,45	5,7	1,8	1,85	conical	45°	45° Chamfer	Hex. 1,20
40.314.004.01-2	1,4	15 N-cm	6,3	1,7	4,6	5,1	1,2	2,1	conical	25°	30° Chamfer	Hex. 1,25
40.314.004.02-2	1,4	15 N-cm	8,4	2,5	5,99	6,7	1,7	2	conical	35°	45° Chamfer	Hex. 1,25
40.314.004.03-2	1,4	15 N-cm	4,3	1,8	2,3	-	2	2	straight	-	45° Chamfer	Hex. 1,25
40.314.005.01-2	1,4	15 N-cm	7,6	3,55	5,17	6	1,6	2,15	conical	25°	45° Chamfer	Hex. 1,27
40.314.005.02-2	1,4	15 N-cm	7,5	2,5	5,5	5,7	1,7	2,1	conical	60°	45° Chamfer	Hex. 1,27
40.314.007.01-2	1,4	15 N-cm	4	1,8	2,01	2,8	1,2	2,2	conical	35°	45° Chamfer	Torx T6
40.314.007.02-2	1,4	15 N-cm	7	2,1	4,75	2,25	0,8	2,1	conical	15°	45° Chamfer	Torx T6
40.314.008.01-2	1,4	15 N-cm	3,5	1,8	2,1	-	1,4	2	straight	-	45° Chamfer	Unigrip
40.314.008.02-2	1,4	15 N-cm	6,7	2,5	4,87	5,3	1,4	1,8	conical	35°	45° Chamfer	Unigrip
40.314.012.01-2	1,4	15 N-cm	4,5	1,7	2,01	2,4	2,1	2,15	conical	45°	45° Chamfer	Star 1,50
40.314.014.01-2	1,4	15 N-cm	4,45	2	2,48	-	1,97	2,16	straight	-	45° Chamfer	Hex. 1,19
40.316.002.01-2	1,6	20 N-cm	7	2,79	4,86	5,44	1,56	2,3	conical	45°	45° Chamfer	Sq. 1,30
40.316.002.02-2	1,6	20 N-cm	9,3	3,3	7,3	-	2	2,3	straight	-	Semi-sphere	Sq. 1,30
40.316.003.01-2	1,6	20 N-cm	8,4	2,5	6,6	-	1,8	2	straight	-	45° Chamfer	Hex. 1,20
40.316.003.02-2	1,6	20 N-cm	10,2	2	7,88	8,2	2	2,2	conical	45°	45° Chamfer	Hex. 1,20
40.316.004.01-2	1,6	20 N-cm	8,6	2,7	6,16	6,9	1,7	2	conical	30°	45° Chamfer	Hex. 1,25
40.316.004.02-2	1,6	20 N-cm	8,8	3	6,73	6,8	1,8	2,1	conical	45°	45° Chamfer	Hex. 1,25
40.316.004.03-2	1,6	20 N-cm	6,9	2,2	5,02	5,2	1,7	1,92	conical	60°	45° Chamfer	Hex. 1,25
40.316.005.01-2	1,6	20 N-cm	7,5	3,6	5,33	5,85	1,65	2,15	conical	30°	45° Chamfer	Hex. 1,27
40.316.005.02-2	1,6	20 N-cm	8,2	3,03	6,25	-	2	2,33	straight	-	45° Chamfer	Hex. 1,27
40.316.005.04-2	1,6	20 N-cm	10,5	2,9	8,15	8,4	2,1	2,1	conical	45°	45° Chamfer	Hex. 1,27

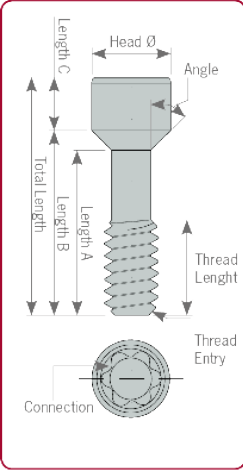
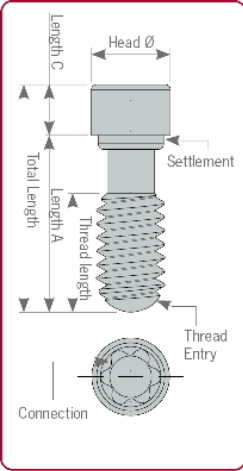


REFERENCE	METRIC	TORQUE	TOTAL LENGTH	THREAD LENGTH	A LENGTH	B LENGTH	C LENGTH	HEAD DIAMETER	SEAT	ANGLE	THREAD ENTRY	CONNECTION
40.316.005.05-2	1,6	20 N-cm	7,6	2,7	5,21	5,5	2,1	2,1	conical	60°	45° Chamfer	Hex. 1,27
40.316.005.06-2	1,6	20 N-cm	3,6	1,8	2,2	-	1,4	2,1	straight	-	45° Chamfer	Hex. 1,27
40.316.005.07-2	1,6	20 N-cm	8,8	2,85	6,73	6,9	1,9	2,15	conical	60	45° Chamfer	Hex. 1,27
40.316.005.08-2	1,6	20 N-cm	9	3,9	0	6,9	2,1	2,18	conical	45°	45° Chamfer	Hex. 1,27
40.316.0 07.01-2	1,6	20 N-cm	7,9	2	5,72	6,9	2,18	2,18	conical	15°	45° Chamfer	Torx T6
40.316.008.01-2	1,6	20 N-cm	7	2,7	5,15	-	1,8	2,3	straight	-	45° Chamfer	Unigrip
40.316.008.02-2	1,6	20 N-cm	7,3	2,7	5,15	5,9	1,4	2,2	conical	35°	45° Chamfer	Unigrip
40.316.012.01-2	1,6	20 N-cm	8	2,65	5,53	6	2	2,15	conical	45°	45° Chamfer	Star 1,50
40.316.014.01-2	1,6	20 N-cm	7,9	2,3	5,42	6,46	1,44	2,2	conical	20°	45° Chamfer	Hex. 1,19
40.317.002.01-2	N1-72	25 N-cm	8,17	3	5,31	5,87	2,3	2,4	conical	45°	45° Chamfer	Sq. 1,30
40.317.004.01-2	N1-72	25 N-cm	7,6	2,8	5,6	5,76	1,84	2,3	conical	70°	45° Chamfer	Hex. 1,27
40.317.004.02-2	N1-72	25 N-cm	7,52	2,2	5,12	5,773	1,75	2,1	conical	30°	45° Chamfer	Hex. 1,25
40.317.005.01-2	N1-72	25 N-cm	7,6	2,5	5,19	5,42	2,18	2,2	conical	60°	45° Chamfer	Hex. 1,27
40.317.005.02-2	N1-72	25 N-cm	7,2	2,4	4,73	5,25	1,95	2,4	conical	45°	45° Chamfer	Hex. 1,27
40.318.002.01-2	1,8	25 N-cm	7	3,2	5,2	-	1,8	2,5	straight	-	45° Chamfer	Sq. 1,30
40.318.002.02-2	1,8	25 N-cm	8,3	2,6	6,6	-	1,7	2,45	straight	-	45° Chamfer	Sq. 1,30
40.318.003.01-2	1,8	25 N-cm	6,8	3,3	5,2	-	1,6	2,3	straight	-	45° Chamfer	Hex. 1,20
40.318.003.02-2	1,8	25 N-cm	8	3,6	6	-	2	2,1	straight	-	45° Chamfer	Hex. 1,20
40.318.004.01-2	1,8	25 N-cm	7,2	4,47	2,3	6,2	1	2,4	conical	30°	45° Chamfer	Hex. 1,25
40.318.004.02-2	1,8	25 N-cm	9,8	5,094	8,3	8,8	1	2,4	conical	30°	45° Chamfer	Hex. 1,25
40.318.004.03-2	1,8	25 N-cm	7,65	3,3	5,17	5,75	1,9	2,4	conical	35°	45° Chamfer	Hex. 1,25
40.318.005.01-2	1,8	25 N-cm	4,5	2,3	2,8	2,9	1,6	2,35	conical	70°	45° Chamfer	Hex. 1,27
40.318.005.02-2	1,8	25 N-cm	7,6	3,8	5,8	6,05	1,55	2,35	conical	50°	45° Chamfer	Hex. 1,27
40.318.006.01-2	1,8	25 N-cm	6	3,18	3,5	3,85	2,15	2,4	conical	45°	45° Chamfer	Hex. 1,50
40.318.007.01-2	1,8	25 N-cm	9,1	4,25	7,22	7,45	1,65	2,18	conical	60°	45° Chamfer	Torx T6
40.318.008.01-2	1,8	25 N-cm	8,3	2,5	6,5	-	1,8	2,45	straight	-	45° Chamfer	Unigrip




STRAIGHT SCREWS TECHNICAL SPECIFICATIONS

REFERENCE	METRIC	TORQUE	TOTAL LENGTH	THREAD LENGTH	A LENGTH	B LENGTH	C LENGTH	HEAD DIAMETER	SEAT	ANGLE	THREAD ENTRY	CONNECTION
40.318.012.01-2	1,8	25 N-cm	7,25	2,4	4,93	5,25	2	2,15	conical	45°	45° Chamfer	Sq. 1,50
40.318.012.02-2	1,8	25 N-cm	8	2,6	5,68	6	2	2,15	conical	45°	45° Chamfer	Sq. 1,50
40.318.013.01-2	1,8	25 N-cm	8	2,5	6,01	6,7	1,3	2,2	conical	30°	45° Chamfer	Hex. 1,00
40.320.002.01-2	2	30 N-cm	5	3,06	3,26	3,5	1,5	2,49	conical	45°	45° Chamfer	Sq. 1,30
40.320.002.02-2	2	30 N-cm	7,45	3	5,7	5,9	1,5	2,4	conical	45°	45° Chamfer	Sq. 1,30
40.320.002.03-2	2	30 N-cm	10,2	3,15	8,4	-	1,8	2,45	straight	-	45° Chamfer	Sq. 1,30
40.320.003.01-2	2	30 N-cm	4,7	2,7	3,33	-	1,37	2,35	straight	-	45° Chamfer	Hex. 1,20
40.320.003.02-2	2	30 N-cm	7	3,25	5	-	2	2,4	straight	-	45° Chamfer	Hex. 1,20
40.320.003.03-2	2	30 N-cm	7,9	3,7	5,55	6,05	1,85	2,4	conical	45°	45° Chamfer	Hex. 1,20
40.320.003.04-2	2	30 N-cm	8,4	2,75	5,68	6,35	2,05	2,3	conical	45°	45° Chamfer	Hex. 1,20
40.320.003.05-2	2	30 N-cm	4,8	3,3	3,65	3,9	0,9	2,45	conical	45°	45° Chamfer	Hex. 1,20
40.320.005.01-2	2	30 N-cm	7,6	3,7	6	-	1,6	2,4	straight	-	45° Chamfer	Hex. 1,27
40.320.005.02-2	2	30 N-cm	10,3	4	8,3	-	2	2,45	straight	-	45° Chamfer	Hex. 1,27
40.320.005.03-2	2	30 N-cm	10,3	3,5	8,3	-	2	2,33	straight	-	45° Chamfer	Hex. 1,27
40.320.005.04-2	2	30 N-cm	10,5	3,06	8,15	8,4	2,1	2,5	conical	45°	45° Chamfer	Hex. 1,27
40.320.007.01-2	2	30 N-cm	6,7	2,25	3,59	5,7	1	2,58	conical	15°	45° Chamfer	Torx T6
40.320.007.02-2	2	30 N-cm	7,4	3,3	6	-	1,4	2,3	straight	-	Semi-sphere	Torx T6
40.320.007.03-2	2	30 N-cm	7,6	3	6,1	6,3	1,3	2,4	conical	45°	Semi-sphere	Torx T6
40.320.007.04-2	2	30 N-cm	4,5	2,96	3,21	3,5	1	2,45	conical	45°	45° Chamfer	Torx T6
40.320.008.01-2	2	30 N-cm	7	3,25	5	-	2	2,4	straight	-	45° Chamfer	Unigrip
40.320.008.02-2	2	30 N-cm	7,3	3	5,8	6,2	1,1	2,5	conical	35°	45° Chamfer	Unigrip
40.320.008.03-2	2	30 N-cm	10	3,6	8,5	-	1,5	2,45	straight	-	45° Chamfer	Unigrip
40.325.002.01-2	2,5	30 N-cm	7,41	3,5	4,75	5,29	2,12	2,87	conical	45°	Semi-sphere	Sq . 1,30
40.325.008.01-2	2,5	30 N-cm	7	2,8	5,6	-	1,4	3,4	straight	-	45° Chamfer	Unigrip

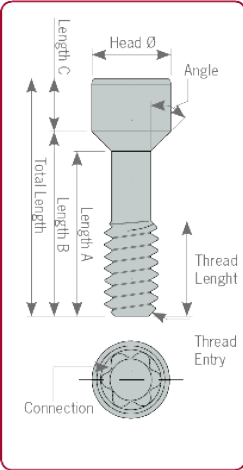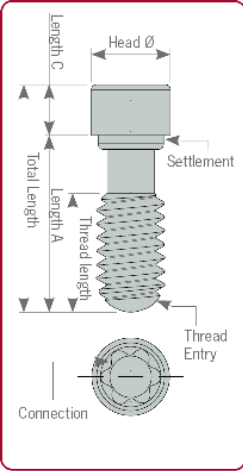

SCREWDRIVERS & STRAIGHT SCREWS

Screwdrivers

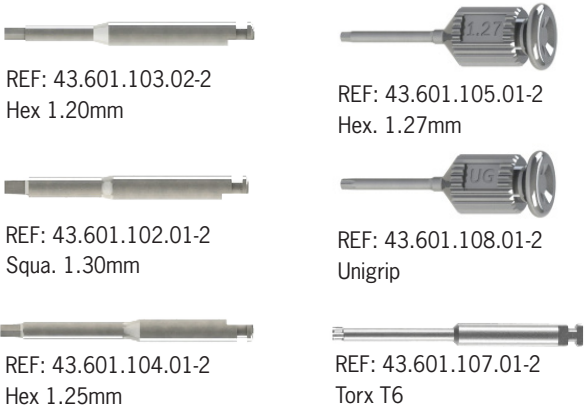


Straight screws cover all the thread metrics available on the market. We have several lengths for each metric to make the adaptation to the milled structures easier. Made of Titanium grade V.




Straight Screws

DYNAMIC SYSTEM SCANBODIES AND COLORS
ACCORDING TO COMPATIBILITY

COMPATIBILITY CODE	MAIN COMPATIBILITY	SCANBODY TYPE	SCANBODY REFERENCE	MIDDLE PIECE	MAGNET SCREW
0002	Biomet 3i Certain RP	HA	52.410.101.01-2		
0007	Astra Evolution 4,2				
0017	MIS C1 RP				
0022	Nobel Biocare Active RP				
0024	Nobel Biocare Branemark RP			N/A	
0030	Osstem Implant TS RP				
0040	Zimmer Screw- Vent 3,5				
0057	Biomet 3i Certain WP				
0005	Astra Lilac	HB	52.410.102.01-2		
0018	MIS C1 WP				
0041	Zimmer Screw- Vent 4,5				
0052	Bego S/RI 4,5				
0091	Astra Evolution 4,8				
0001	Biomet 3i Certain NP	HC	52.410.103.01-2		
0004	Astra Aqua				
0021	Nobel Biocare Active NP				
0023	Nobel Biocare Branemark NP			N/A	
0029	Osstem Implant TS Mini				
0038	Xive S 3,4				
0083	Klockner Vega RV				

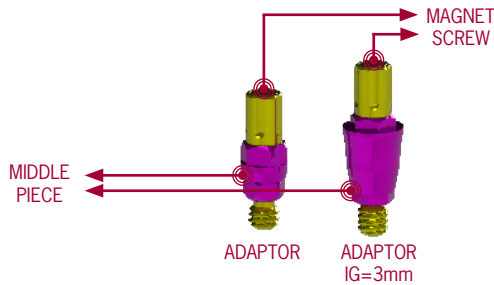


COMPATIBILITY CODE	MAIN COMPATIBILITY	SCANBODY TYPE	SCANBODY REFERENCE	MIDDLE PIECE	MAGNET SCREW
0003	Biomet 3i Osseotite NP	HD	52.410.104.01-2	N/A	
0015	Megagen AnyRidge RP				
0006	Astra Evolution 3,6	HE	52.410.105.01-2		
0019	MIS M4 NP				
0044	Keystone Prima NP				
0075	Ankylos				
0082	Klockner Vega NV				
0008	Astra Evolution Uni Abutment	HF	52.408.113.01-2	N/A	
0009	BTI External Connection NP	HG	52.410.114.01-2	N/A	
0039	Xive S 3,8				
0187	Bego Mini			N/A	
0049	Bego RS/RSX 3	HH	52.410.116.01-2		
0050	Bego S/RI 3,25-3,75	HI	52.410.117.01-2		
0085	Xive S 4,5				
0125	Medentis ICX-Templant 4,1				
0167	Lasak Bionoq QR				
0169	Alphabio Conical Standard Connection	HJ	52.410.118.01-2		
0051	Bego S/RI 4,1				
0045	Keystone Prima RP				
0058	Biomet 3i Osseotite WP			N/A	

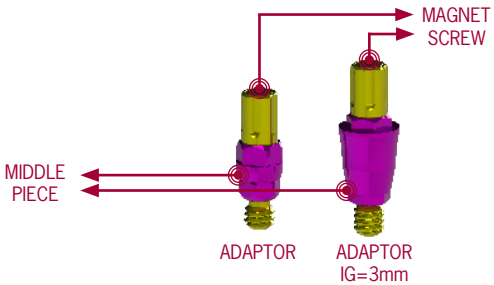


DYNAMIC SYSTEM SCANBODIES AND COLORS
ACCORDING TO COMPATIBILITY

COMPATIBILITY CODE	MAIN COMPATIBILITY	SCANBODY TYPE	SCANBODY REFERENCE	MIDDLE PIECE	MAGNET SCREW
0060	BTI External Connection WP	HM	52.410.122.01-2	N/A	
0047	Neoss ProActive 3,4	HN	52.409.123.01-2		
0048	Neoss ProActive 4,1				
0151	BTI Multi-IM Universal RP			N/A	
0080	Zimmer Screw-Vent 5,7	HO	52.410.124.01-2		
0046	Keystone Prima WP	HP	52.410.125.01-2		
0061	Nobel Biocare Branemark WP			N/A	
0124	Nobel Biocare Active WP				
0081	Bego S/RI 5,50	HR	52.410.126.01-2		
0014	DIO UF NP	HS	52.410.128.01-2		
0090	Astra Evolution 3,0				
0102	Biohorizons 3,0				
0109	Astra Yellow				
0136	Alphabio Conical Hex. Connection				
0159	Nobel Biocare Active 3,0				
0164	Biotech Dental Kontakt 3.0				
0092	Astra Evolution 5,4	HT	52.410.129.01-2		
0025	Nobel Biocare Multi Unit RP	MA	52.410.111.01-2	N/A	
0020	MIS Multi Unit St	MB	52.408.112.01-2	N/A	
0025	Nobel Biocare Multi Unit RP			N/A	
0163	Anthogyr Multi-Unit 4,8			N/A	
0181	Paltop MU			N/A	

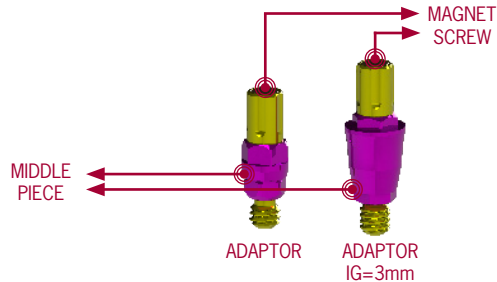


COMPATIBILITY CODE	MAIN COMPATIBILITY	SCANBODY TYPE	SCANBODY REFERENCE	MIDDLE PIECE	MAGNET SCREW
0037	Straumann Internal Octagon 4,8	OA	52.410.110.01-2	N/A	
0074	Straumann Synocta RP				
0096	Straumann Internal Octagon 6,5				
0054	Klockner Essential Cone 4,5	OB	52.410.119.01-2		
0016	MIS C1 NP	SA	52.410.106.01-2		
0033	Straumann Bone Level NP				
0035	Straumann Bone Level RP	SB	52.410.107.01-2		
0010	BTI Internal Connection RP	SC	52.410.115.01-2		
0160	Straumann Tissue Level NNC	SD	52.410.131.01-2		
0011	Camlog Screw-Line 3,8	TA	52.410.108.01-2		
0026	Nobel Biocare Replace NP				
0120	Conelog 3,8				
0012	Camlog Screw-Line 4,3	TB	52.410.109.01-2		
0027	Nobel Biocare Replace RP				
0028	Nobel Biocare Replace WP				
0121	Conelog 4,3				
0129	Nobel Biocare Replace 6,0	TC	52.410.130.01-2		
0149	Anthogyr Axiom REG/PX XNP	TD	52.410.132.01-2		
0162	Anthogyr Axiom REG/PX WP				
0161	Anthogyr Axiom REG/PX RP				
0165	Biotech Dental Kontakt RP				

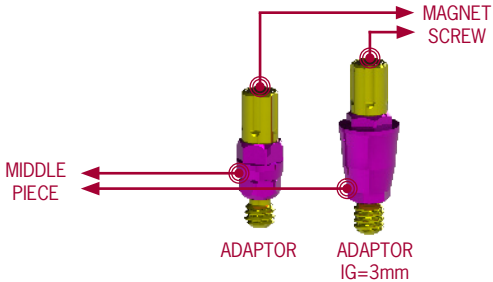

MAIN COMPATIBILITY	REFERENCE	CUTTING DIAMETER	SEAT	CUTTING LENGTH	USEFUL LENGTH (max. drilling depth)	STEM CUTTING DIAMETER	SUPPORT DIAMETER (SHANK)	TOTAL LENGTH
		Øc	α	Lc	Lu	Øv	Øs	Lt
BEGO RS/RXS 3* ASTRA EVOLUTION 3.0* *Only for titanium and soft materials	33.325.472.01-2	1,4	25	0,4	4,7	0,5	3	50
	33.425.472.01-2	1,4	25	0,4	4,7	0,5	4	50
	33.625.472.01-2	1,4	25	0,4	4,7	0,5	6	50
STRAUMANN BONE LEVEL NP STRAUMANN BONE LEVEL RP MEDENTIS ICX TEMPLANT 4,1 STRAUMANN SYNOCTA 3.5	33.315.804.01-2	1,6	15	0,7	8	0,65	3	50
	33.415.804.01-2	1,6	15	0,7	8	0,65	4	50
	33.615.804.01-2	1,6	15	0,7	8	0,65	6	50
ANTHOGYR AXIOM RG/PX XNP ANTHOGYR AXIOM RG/PX RP ANTHOGYR AXIOM RG/PX WP	33.320.704.01-2	1,6	20	0,7	7	0,8	3	50
	33.420.704.01-2	1,6	20	0,7	7	0,8	4	50
	33.620.704.01-2	1,6	20	0,7	7	0,8	6	50
ASTRA EVOLUTION 3.6 ANKYLOS ALPHABIO CONICAL STANDARD CONNECTION LASAK BIONIQ QR NEODENT GM	33.330.734.01-2	1,6	30	0,7	7,3	0,8	3	50
	33.430.734.01-2	1,6	30	0,7	7,3	0,8	4	50
	33.630.734.01-2	1,6	30	0,7	7,3	0,8	6	50
NOBEL BIO CARE ACTIVE NP NOBEL BIO CARE ACTIVE 3.0 LASAK BIONIQ QN	33.335.754.01-2	1,6	35	0,7	7,5	0,65	3	50
	33.435.754.01-2	1,6	35	0,7	7,5	0,65	4	50
	33.635.754.01-2	1,6	35	0,7	7,5	0,65	6	50
OSSTEM TS NP CAMLOG SCREW LINE 3.8 NP CAMLOG SCREW LINE 4.3 RP KLOCKNER VEGA NV XIVE S 3,4 BIOTECH DENTAL KONTAKT XNP BIOTECH DENTAL KONTAKT RP DIO UF NP CAMLOG SCREW-LINE 3,3	33.345.804.01-2	1,6	45	0,7	8	0,65	3	50
	33.445.804.01-2	1,6	45	0,7	8	0,65	4	50
	33.645.804.01-2	1,6	45	0,7	8	0,65	6	50
MIS C1 NP MIS M4 NP CONOLOG 3,8 CONOLOG 4,3 ASTRA YELLOW ALPHABIO CONICAL HEX CONNECTION	33.360.754.01-2	1,6	60	0,7	7,5	0,65	3	50
	33.460.754.01-2	1,6	60	0,7	7,5	0,65	4	50
	33.660.754.01-2	1,6	60	0,7	7,5	0,65	6	50
BIOMET 3i CERTAIN NP ASTRA AQUA	33.390.754.01-2	1,6	90	0,7	7,5	0,65	3	50
	33.490.754.01-2	1,6	90	0,7	7,5	0,65	4	50
	33.690.754.01-2	1,6	90	0,7	7,5	0,65	6	50
ASTRA EVOLUTION 4.2	33.350.775.01-2	1,7	50	0,7	7,7	0,8	3	50
	33.450.775.01-2	1,7	50	0,7	7,7	0,8	4	50
	33.650.775.01-2	1,7	50	0,7	7,7	0,8	6	50
BIOMET 3i CERTAIN RP NOBEL BIO CARE BRANEMARK NP NOBEL BIO CARE REPLACE NP MEGAGEN ANYRIDGE RP BIOMET 3i CERTAIN WP	33.390.805.01-2	1,7	90	0,7	8	0,65	3	50
	33.490.805.01-2	1,7	90	0,7	8	0,65	4	50
	33.690.805.01-2	1,7	90	0,7	8	0,65	6	50
BEGO S/Ri 3.25-3.75 BEGO S/Ri 4.1 BEGO S/Ri 4.5 BEGO S/Ri 5,50 STRAUMANN SCREW-RETAINED NC/RC BEGO MULTIPLUS	33.335.676.01-2	1,8	35	1	6,7	0,9	3	50
	33.435.676.01-2	1,8	35	1	6,7	0,9	4	50
	33.635.676.01-2	1,8	35	1	6,7	0,9	6	50
KLOCKNER ESSENTIAL CONE 4.5 DIRECTO IMPLANTE KLOCKNER ESSENTIAL CONE 4.5 OCTACONE 12° KLOCKNER ESSENTIAL CONE 4.5 OCTACONE 25° KLOCKNER VEGA RV XIVE S 3,8 XIVE S 4,5 BIOHORIZONS 3.0 STRAUMANN SYNOCTA 6,5	33.345.856.01-2	1,8	45	1	8,5	0,9	3	50
	33.445.856.01-2	1,8	45	1	8,5	0,9	4	50
	33.645.856.01-2	1,8	45	1	8,5	0,9	6	50

DYNAMIC MILLING TOOL SPECIFICATIONS

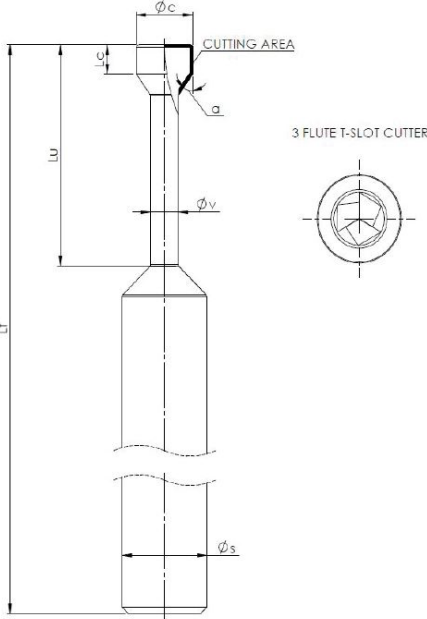

MAIN COMPATIBILITY	REFERENCE	CUTTING DIAMETER	SEAT	CUTTING LENGTH	USEFUL LENGTH (max. drilling depth)	STEM CUTTING DIAMETER	SUPPORT DIAMETER (SHANK)	TOTAL LENGTH
		Øc	α	Lc	Lu	Øv	Øs	Lt
MIS C1 RP PALTOP UNIVERSAL MULTI UNIT MIS C1 WP S&M PREMIUM KHONO 3,3 S&M PREMIUM KHONO 3,8 S&M OUTLINK 3,3 S&M OUTLINK 4,1 S&M PREMIUM KHONO 4,25 BREDENT SKY NP BREDENT SKY RP ADIN TOUAREG/CLOSEFIT NP ADIN TOUAREG/CLOSEFIT UNP	33.360.756.01-2	1,8	60	1	7,5	0,9	3	50
	33.460.756.01-2	1,8	60	1	7,5	0,9	4	50
	33.660.756.01-2	1,8	60	1	7,5	0,9	6	50
ZIMMER SCREW-VENT 3.5 ZIMMER SCREW-VENT 4.5 ASTRA EVOLUTION UNIT ABUTMENT ZIMMER TYPE 5,7	33.370.716.01-2	1,8	70	1	7,1	0,9	3	50
	33.470.716.01-2	1,8	70	1	7,1	0,9	4	50
	33.670.716.01-2	1,8	70	1	7,1	0,9	6	50
NOBEL BIO CARE BRANEMARK RP NOBEL BIO CARE MULTI-UNIT RP BIOMET 3i OSSEOTITE NP BTI EXTERNAL CONNECTION NP BTI INTERNAL CONNECTION RP MIS MULTI-UNIT ST KEYSTONE PRIMA NP KEYSTONE PRIMA RP KEYSTONE PRIMA WP NEOSS PROACTIVE 3,4 NEOSS PROACTIVE 4,1 BIOMET 3i OSSEOTITE WP BTI EXTERNAL CONNECTION WP BTI MULTIM UNIVERSAL RP ANTHOGYRD MULTI-UNIT 4.8 BEGO MINI BTI INTERNAL WP LASAK MULTI-UNIT QN/QR SIC SICACE 3,3 SIC SICACE 4,2	33.390.716.01-2	1,8	90	1	7,1	0,9	3	50
	33.490.716.01-2	1,8	90	1	7,1	0,9	4	50
	33.690.716.01-2	1,8	90	1	7,1	0,9	6	50
STRAUMANN INTERNAL OCTAGON RP STRAUMANN INTERNAL OCTAGON 6,5	33.315.708.01-2	2	15	1	7	1	3	50
	33.415.708.01-2	2	15	1	7	1	4	50
	33.615.708.01-2	2	15	1	7	1	6	50
STRAUMANN SYNOCTA RP	33.330.708.01-2	2	30	1	7	1	3	50
	33.430.708.01-2	2	30	1	7	1	4	50
	33.630.708.01-2	2	30	1	7	1	6	50
NOBEL BIO CARE ACTIVE RP NOBEL BIO CARE ACTIVE WP	33.335.758.01-2	2	35	1	7,5	1	3	50
	33.435.758.01-2	2	35	1	7,5	1	4	50
	33.635.758.01-2	2	35	1	7,5	1	6	50
OSSTEM TS RP CAMLOG SCREW-LINE 5,0 CAMLOG SCREW-LINE 6,0	33.345.808.01-2	2	45	1	8	1	3	50
	33.445.808.01-2	2	45	1	8	1	4	50
	33.645.808.01-2	2	45	1	8	1	6	50
NOBEL BIO CARE REPLACE RP ASTRA LLAC NOBEL BIO CARE REPLACE WP ASTRA EVOLUTION 4.8 NOBEL BIO CARE BRANEMARK WP ASTRA EVOLUTION 5.4 NOBEL BIO CARE REPLACE 6.0	33.390.958.01-2	2	90	1	9,5	1	3	50
	33.490.958.01-2	2	90	1	9,5	1	4	50
	33.690.958.01-2	2	90	1	9,5	1	6	50

Reference code:

Cutting seat Cutting diameter
code
33.445.804.01-2
Shank Useful length



DMTONE
DYNAMIC MILLING TOOL

SCREWDRIVER ADAPTOR

Screwdriver for the Dynamic µScanbody System

Ref. 43.621.410.01-2
Screwdriver with manual handle
Standard length: 21mm



Ref. 43.624.410.01-2
Contra-angle
Length: 24mm



Ref. 43.630.410.01-2
Contra-angle
Length: 30mm



Ref. 43.621.415.01-2
Tiny
Screwdriver with manual handle
Length: 21mm



Ref. 43.620.411.01-2
Multi Unit
Manual handle
Length: 20 mm



COMPLEMENTS

Manual handle

Made of stainless steel.
They are used to connect screwdriver bits with the contra-angle connection



Large manual handle for laboratory Ref. 49.601.000.03-2
Ideal to manipulate models in the laboratory.
Length: 55.65mm.



Manual handle for clinic

Ref. 49.601.000.01-2
Clinic handle: used to position the prosthesis in the mouth prior to torque control in the clinic.
Length: 15.65mm.



Manual torque wrench adapter prosthetic

Piece to connect the screwdriver with contra-angle connection to the torque wrench.



Universal Manual torque wrench adapter
Ref. 49.604.000.05-2
4mm Square connection



Straumann Manual torque wrench adapter
Ref. 49.604.000.07-2
Straumann connection



Nobel Biocare Manual torque wrench adapter
Ref. 49.604.000.08-2



Universal manual torque wrench prosthetic

Ref. 11.990.990.07-2
Torque wrench.
4mm square connection.
Torque 10-35N.c


IDENTIFICATION PRODUCT

The label accompanying all Dynamic Abutment® Solutions products contains all the information the user requires.

The product label contains detailed information of the contents of the blister pack. The symbols found on the

identity labels correspond to the international product identification standards.

All products are supplied with their corresponding instructions for use which include an explanation of each of the symbols found on the product label.

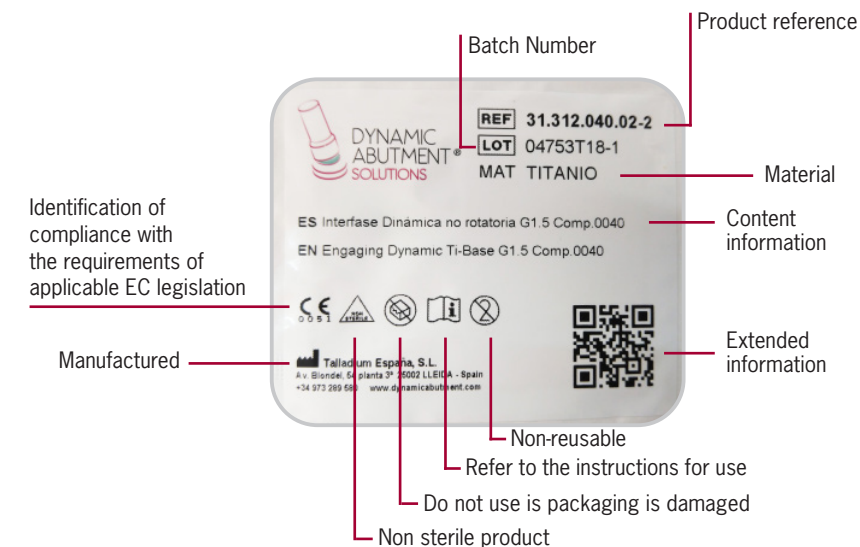

SECURITY & TRACEABILITY

All of our products are patented and manufactured under very strict quality guidelines.

With the 3.0 Dynamic System, we provide a card for the patient and labels for the laboratory and the clinic to identify the position in Dynamic System is located.

We exercise complete control over the traceability of our products to fulfil the current health legislation.

This helps repositioning the material and inform about the importance of using the appropriate tools when handling the Dynamic System components.



TALLADIUM GUARANTEE

TERMS AND CONDITIONS

These guarantee terms and conditions (“T&C”) cover the entire range of Talladium products (“Products”), manufactured by TALLADIUM ESPAÑA S.L. and distributed by Geoda Medical S.L. or official dealers. The guarantee described in these T&C is exclusively in benefit of the clinician (“Clinician”) and of the dental technician (“Technician”) and not for the benefit of third parties or institutions, including patients.

GUARANTEE PERIOD

TALLADIUM ESPAÑA S.L. offers a lifelong guarantee for its entire range of products starting from the date of issue of the invoice.

GUARANTEE SCOPE

Subject to the limitations and exceptions described in these T&C, TALLADIUM ESPAÑA S.L. will offer the following benefits:

QUALITY: If there are defects in the materials or in the manufacturing of the Product, TALLADIUM ESPAÑA S.L. will replace the Product with no additional cost.

SAFETY: If, having complied with all the product indications, the prosthesis should have to be made again, due to a fault in the Dynamic Abutment® or Dynamic Titanium Base® system, TALLADIUM ESPAÑA S.L. will replace the abutments and screws necessary to remake the prosthesis, as well as the costs derived from its manufacturing.

In case of having used our products and having complied with all the product indications, the implants suffer any damage, TALLADIUM ESPAÑA S.L. will pay the cost of the implants. This coverage will only be valid during the first 6 months after the collocation of the prosthesis which includes our products.

CLAIM REQUIREMENTS AND PROCEDURE

To receive the benefits indicated in these T&C, the treating Clinician must satisfy the following requirements:

- a) The claim must be notified to TALLADIUM ESPAÑA S.L. within (30) days since the date the claimed defect was detected.
- b) This requires that the Clinician or Technician must contact the customer service department by telephone or by e-mail to make the claim.
- c) A claim form will be completed, which, together with a document or report which justifies the faulty Product and the faulty Product itself, will be sent by the customer to TALLADIUM ESPAÑA S.L. offices, within the previously indicated period.
- d) Clinicians or Technicians presenting a claim in agreement with these T&C must be up to date in any payments owing to TALLADIUM ESPAÑA S.L. or to any of its subsidiaries, at the time when the claim form is presented.
- e) All the use procedures of our Products must be carried out in agreement with the instructions of TALLADIUM ESPAÑA S.L. as well as in accordance with commonly accepted dentistry practices.
- f) The expenses derived from this procedure will be assumed by the customer. The return shipping costs will be assumed by TALLADIUM ESPAÑA S.L. in all those cases covered by these T&C.

Regardless of the guarantee rights, claims should be notified as soon as possible in order to comply with regulatory requirements.

GENERAL LIMITATIONS OF THIS GUARANTEE

With the exception of the guarantee described in these T&C, neither TALLADIUM ESPAÑA S.L. nor its representatives, nor third parties manufacturing or distributing the Products, represent or offer a guarantee, agreement or any other express or implicit, oral or written, commitment, with respect to the Products (without limitation), including guarantees involved in the marketing, durability or suitability for individual uses or purposes.

In addition and within the maximum extent permitted by the relative law, TALLADIUM ESPAÑA S.L. rejects (on its own behalf, and on behalf of its representatives and third parties that manufacture or distribute Products) any responsibility with respect to any direct or indirect damage caused, which may result from or be a consequence of the design, composition of the dental prosthesis into which the Products are integrated.

GUARANTEE EXCLUSIONS

TALLADIUM ESPAÑA S.L. limits this guarantee to:

- Transformed abutments that form part of the dental prosthesis. But not the screws used to anchor them.
- Clinical screws that have been in the mouth for more than 2 years.

AMENDMENT OR SUSPENSION OF THE GUARANTEE

TALLADIUM ESPAÑA S.L. reserves the right to amend or withdraw these T&C at any time and without prior notification. Any modification or suspension shall not affect products already placed in patients.

Ed.2019-01

NOTES

NOTES



VIRGINIA WOOLF, 17 · 25005 · LLEIDA (SPAIN)
INTERNATIONAL +34 973 289 580
das@dynamicabutment.com

SPAIN +34 973 289 580
spain@dynamicabutment.com

www.dynamicabutment.com



